

Sicherheit in Technik und Chemie



CERTIFIED REFERENCE MATERIALS

CATALOGUE 2024

**Certified
Reference Materials
Catalogue**

Published by:
Bundesanstalt für Materialforschung
und -prüfung (BAM)
Unter den Eichen 87
12205 Berlin, Germany
Mailing address: 12200 Berlin, Germany
Phone: +49 30 8104-0
Fax: +49 30 8104-7-2222
Email: info@bam.de
Internet: <https://www.bam.de>

Berlin, January 2024

Edited by: Dr. S. Recknagel

Printed by:
Bundesanstalt für Materialforschung
und -prüfung (BAM)
Unter den Eichen 87
12205 Berlin

Foreword

Certified Reference Materials, as defined in the ISO Guide 30 and the International Vocabulary of Metrology (VIM), can act as traceability links to the International System of Measurement (SI). By application, e.g. of a CRM whose matrix and analyte levels match those of the samples under investigation as closely as possible, the analyst is able to assure himself that his measurements have been properly carried out to the required level of accuracy.

The BAM Federal Institute for Materials Research and Testing has a long tradition in the production of Certified Reference Materials. Starting in 1912 with a "Normal Steel" for the determination of carbon, the development of new CRMs has increased continuously. One year later 8 steel samples with different carbon contents were available. The development continued with the participation of regional German material research and testing institutes as well as industry (1957). In 1968 within the framework of EURONORM, the first European CRMs in the field of iron and steel were issued (see page 10). In 2003 the European Reference Materials (ERM®) initiative was launched by BAM together with EUROPEAN COMMISSION JRC and LGC to create a European brand of CRMs of high metrological quality.

Since 2016 BAM is accredited by DAkkS as a producer of RM in accordance with ISO 17034 (General requirements for the competence of reference material producers). The scope of accreditation comprises certified reference materials in the form of non-ferrous metals and alloys, ceramics and glass, soils and sediments, food, ethanol/water solutions, aqueous solutions of stable isotopes, lubricants and fuels as well as porous materials.

Today a large range of ferrous and non-ferrous CRMs together with environmental CRMs and CRMs for engineering materials are offered in our new catalogue.

The catalogue provides technical and general ordering information for the CRMs currently available from the BAM Federal Institute for Materials Research and Testing.

BAM holds an accreditation as a reference material producer according to ISO 17034. This accreditation is valid only for the scope as specified in the certificate D-RM-11075-01-00.

DAkkS is a signatory of the multilateral agreement (MLA) between EA, ILAC and IAF for mutual acceptance.



Reference material (RM): material, sufficiently homogeneous and stable with respect to one or more specified properties, which has been established to be fit for its intended use in a measurement process

Note 1 RM is a generic term.

Note 2 Properties can be quantitative or qualitative, e.g. identity of substances or species.

Note 3 Uses may include the calibration of a measurement system, assessment of a measurement procedure, assigning values to other materials, and quality control.

Note 4 A single RM cannot be used for both calibration and validation of results in the same measurement procedure.

Note 5 VIM has an analogous definition (ISO/IEC Guide 99:2007, 5.13), but restricts the term "measurement" to apply to quantitative values and not to qualitative properties. However, Note 3 of ISO/IEC Guide 99:2007, 5.13, specifically includes the concept of qualitative attributes, called "nominal properties".

Certified reference material (CRM): reference material characterized by a metrologically valid procedure for one or more specified properties, accompanied by a certificate that provides the value of the specified property, its associated uncertainty, and a statement of metrological traceability

Note 1 The concept of value includes qualitative attributes such as identity or sequence. Uncertainties for such attributes may be expressed as probabilities.

Note 2 Metrologically valid procedures for the production and certification of reference materials are given in, among others, ISO Guides 34 and 35.

Note 3 ISO Guide 31 gives guidance on the contents of certificates.

Note 4 VIM has an analogous definition (ISO/IEC Guide 99:2007, 5.14).

Note: In this document the comma (and not the dot) is used as a decimal separator.

Ordering BAM reference materials

General

Purchase orders for BAM-CRMs should be directed to:

**Bundesanstalt für Materialforschung
und -prüfung (BAM)
Fachbereich 1.6 Anorganische Referenzmaterialien
Richard-Willstaetter-Str. 11
12489 Berlin, Germany**

Phone: +49 30 8104-2061

Fax: +49 30 8104-72061

Email: sales.crm@bam.de

Webshop: <https://www.webshop.bam.de>

Terms of delivery:

Prices include transport service by mail.

Terms of delivery: free delivery:

BAM usually delivers via DHL.

If another courier or carrier etc. is desired, then the customer bears the costs at the point of destination.

BAM will assume no further costs.

Orders shipping to destinations outside Europe or bulky parcels is charged additionally (flat rate is deducted).

Your products will be packed and shipped asap. Shipment will be performed by standard mail service. Duration of mail delivery cannot be guaranteed by BAM because of different national delivery services.

Content

Certified.....	4
Reference Materials	4
Catalogue	4
Iron and steel products	7
EURONORM certified reference materials for the chemical analysis of iron and steel products.....	8
Unalloyed steels	10
Pure iron.....	11
Highly alloyed steels	16
Special alloys	20
Cast irons	21
Ferro alloys.....	22
Ores, iron oxide	23
Ceramic materials.....	25
Molybdenum oxide	25
Slags.....	26
Steels with certified oxygen and nitrogen content	26
Setting-up sample for spectrometric analysis of low alloyed steels	27
Steel with certified hydrogen content.....	27
Non ferrous metals and alloys.....	29
Aluminium	30
Copper	35
Tin-lead solder	42
Precious metal alloys	43
Zinc.....	43
Zinc-alloy	43
Lead-alloys, discs	44
Special materials Glass	47
High tech ceramics	49
Boron carbide powder.....	49
Boron nitride powder Silicon nitride powder	49
Yttrium stabilized zirconium oxide	50
Silicon carbide powder	50
Tungsten metal powder	51
Niobium pentoxide	52
Niobium carbide powder	52
Li-NMC 111 Cathode Material	53
Graphite powder	54
Multielement-glass.....	55
Iron in flat glass.....	55
Borosilicate glass.....	56
Acrylonitrile-butadiene-styrene copolymerisate (ABS).....	56
Pure substances	57
Platinum group elements (PGE) in used automobile catalyst	59
Electronic scrap.....	59
Environment	61
Calibration standards "Ethanol in Water" □	62
Calibration standard for the determination of mineral oil hydrocarbons in environmental matrices using gas chromatography	62
BAM-K010g□ Diesel oil/lubricating oil (1:1)	62
BAM-K008a□ Diesel oil	62
BAM-K009a□ Lubricating oil.....	62
Sulfur in petrol.....	63
Adsorbed organically bound halogens (AOX) in soil	63
Adsorbed organically bound halogens (AOX) in sludge	63

Mineral oil contaminated sediment and soil	64
Polychlorinated biphenyls in soil	64
Pentachlorophenol (PCP) in wood	64
Trace elements in wood	64
Trace elements in contaminated river sediment	65
Total cyanide in soil	65
Trace elements in sewage sludge ash	66
Food	67
Polycyclic aromatic hydrocarbons in olive oil	68
Acrylamide in crispbread	68
Acrylamide in rusk	68
Fusarium mycotoxins in wheat flour	68
Zearalenone in maize germ oil	68
T-2 and HT-2 toxin in oat flakes	68
Cadmium and Acrylamide in Cocoa	68
Consumer products	69
Polycyclic aromatic hydrocarbons in rubber toy	70
Gas mixtures	71
Certified reference gas mixtures	72
Certified reference gas mixtures for gas calorimeters [□]	76
Certified reference gas mixtures for process gas chromatographs [□]	76
Binary certified reference gas mixtures	83
Multicomponent certified reference gas mixtures	83
Elastomeric materials	85
Standard reference elastomers (SRE) from vulcanized rubbers	86
Optical properties	89
X-ray film step tablet	90
Calibration kit Spectral fluorescence standards	90
Fluorescence Quantum Yield Standards	90
Porous reference materials	91
CRMs for the gas adsorption method	92
CRMs for the mercury intrusion method	93
Layer and surface reference materials	97
EDS-TM002 test material and optional software package for the performance check of an energy dispersive X-ray spectrometer (EDS)	98
Particle size distribution	101
CRM for particle size distribution by laser diffraction methods according to ISO 13320	102
Polymeric reference materials	103
CRMs for the determination of the molecular weight	104
Microplastic	105
Isotopic reference materials	107
CRMs certified for the isotopic composition of boron	108
CRM certified for the isotopic composition of cadmium	110
CRM certified for the mass fraction and the isotopic composition of palladium	111
CRM certified for the mass fraction and the isotopic composition of platinum	112
CRM certified for the isotopic composition of lead	113
CRM certified for the isotopic composition of magnesium	114
Nano materials	115
BAM-N008	116
BAM-N012	116
Experts	117

Iron and steel products

EURONORM certified reference materials for the chemical analysis of iron and steel products

EURONORM certified reference materials are prepared by the EURONORM-CRM producers group in a collaboration between the producing organizations in:

France: ArcelorMittal Maizières (Institute de Recherches de la Sidérurgie (IRSID))

Federal Republic of Germany: Bundesanstalt für Materialforschung und -prüfung (BAM),

Sweden/Finland: Jernkontoret, Oy Narema Ab.

Starting in 1968 EURONORM-CRMs have been analysed by laboratories in the European Community (EC) and further European countries. These samples are indicated by an asterisk in the tables. A number of former national CRMs are also listed in the tables. After examination by laboratories in the EC they have been accepted as EURONORM-CRMs.

Approximately 20 laboratories take part in the analysis. Each laboratory is requested to analyse the elements to be determined four times. A statistical evaluation of the laboratory mean values is carried out with respect to their normal distribution and the identification of any outlying values.

The finely divided EURONORM-CRMs are supplied in glass bottles containing 100 g. Some EURONORM-CRMs are also available in solid form (discs). Samples in the form of chips, pins and balls with certified oxygen and nitrogen content are also available.

This catalogue represents European CRMs of German origin. For CRMs of British, Swedish and French origin please contact the above mentioned producers. Details of all ECRMs are given in CEN-Report CR 10317 and CEN TR 10350 (ECSC), both of which are available from the national standards body in your country.

Types of material

The following types of material are available as EURONORM-CRM:

Unalloyed steels (0), alloyed steels (1), highly alloyed steels (2), special alloys (3), cast iron (4), ferro-alloys (5), ores (6), ceramics (7) and slags (8).

Our system of numbering of the samples allows an easy orientation about the type of material. The first digit of the sample number shows the type of material (0 - unalloyed steel, 1 - low alloyed steel, 2 - highly alloyed steel etc.). The second and third digit characterizes the single sample. Another digit, separated by a hyphen gives the number of editions of the material.

Content of the certificate

On the head of the certificate the EURONORM-number and the type of material of the sample is given. The mean values of the laboratories involved in the certification campaign are given in a table together with indicative values. The mean values of the accepted data sets, their standard deviations and the standard deviations of the laboratories are also given in the table. The sign "-" in the table stands for an outlier pointed out by statistical tests. The certified values are given in a second table together with their uncertainties (95%-level) or standard deviations. Additionally the following information are given: The owner of the material, a characterization of the sample (e.g. grain size, dimensions of compact samples), the laboratories involved in the certification campaign, the analytical methods used for element determination, sources for getting additional information published by ECISS/EGKS.

The following information are given in the tables:

Indicative values (not certified) are given in parentheses.

Authentic for the certified element contents are only the values given in the certificates, not the values given in this catalogue.

Samples for the determination of nitrogen and oxygen (N-O-materials)

Three different types of material are available:

Unalloyed steel: the pin-shaped material (100 mm long, 8 mm in diameter) forms an iron oxide coating. Before analysis this layer has to be removed by turning and care has to be taken to prevent a reoxidation of the cleaned surface.

Highly alloyed stainless steel: after formation of a reproducible and constant oxide layer the chipped material is protected (passivated) against further oxidation. There is no need for sample pretreatment.

Highly alloyed steel pins (6 mm long, 4 mm in diameter). Cleaning with acetone is recommended.

Samples for optical emission and X-ray fluorescence spectrometry

The samples are in form of discs (cylinders of 36 to 41 mm diameter and 20 to 35 mm height) and normally also available in form of chips. The samples 035-2, 284-3, and 290-1/291-1 are prepared by hot isostatic pressing (HIP) of powder which was atomized from the melt and solidified in inert gas giving a material of high homogeneity.

Unalloyed steels

Mass fraction in % ± standard deviation

CRM-No.	D 030-4	D 031-3	D 032-2	D 035-2 ¹⁾	D 036-1
Year of issue	1973	1972	1968	1998	1968
Chips, powder	•	•	•	•	•
Disc				•	
C	0,456 ± 0,004	0,055 ± 0,002	0,271 ± 0,007	1,277 ± 0,005	0,858 ± 0,008
Si	0,318 ± 0,007	0,037 ± 0,004	0,282 ± 0,007	0,216 ± 0,004	0,194 ± 0,005
Mn	0,603 ± 0,004	0,329 ± 0,007	0,556 ± 0,008	0,305 ± 0,002	0,327 ± 0,010
P	0,018 ± 0,002	0,014 ± 0,001	0,0129 ± 0,0007	0,0038 ± 0,0003	0,0074 ± 0,0009
S	0,021 ± 0,002	0,021 ± 0,001	0,0254 ± 0,0010	0,0111 ± 0,0003	0,0095 ± 0,0009
Cr	0,117 ± 0,004	–	(0,088)	0,0104 ± 0,0003	(0,091)
Mo	–	–	–	0,0056 ± 0,0002	–
Ni	0,042 ± 0,002	–	(0,040)	0,0190 ± 0,0004	(0,058)
Al_{total}	0,042 ± 0,006	0,054 ± 0,002	–	0,0193 ± 0,0005	(0,015)
Al_{insol.}	–	–	–	–	–
Al_{acid-sol.}	–	–	–	0,0177 ± 0,0004	–
As	0,012 ± 0,002	0,013 ± 0,002	0,020 ± 0,002	0,0017 ± 0,0001	0,0233 ± 0,0007
Cu	0,061 ± 0,002	0,020 ± 0,002	0,085 ± 0,002	0,0085 ± 0,0002	0,065 ± 0,005
N	0,0051 ± 0,0003	0,0050 ± 0,0004	0,0044 ± 0,0009	0,0230 ± 0,0004	0,0100 ± 0,0008
Nb	–	–	–	–	–
Pb	–	–	–	–	–
Sn	0,0055 ± 0,0007	–	(0,006)	–	(0,006)
Ti	–	–	–	0,0030 ± 0,0001	–
V	–	–	–	–	(0,019)
Te	–	–	–	–	–

(Values in parentheses are indicative values)

- continued -

¹⁾ Powdered material, produced by atomization of the melt

Unalloyed steels (continued)

CRM-No.	D 042-1	D 079-2	D 082-1	D 083-1	D 083-2
Year of issue	1972	1989	1976	1978	2017
Chips, powder	•	•	•	•	•
Disc					•
C	0,108 ± 0,003	0,596 ± 0,006	0,415 ± 0,003	0,0262R ± 0,0004 ⁺	0,0315 ± 0,0006
Si	0,037 ± 0,005	0,247 ± 0,006	0,235 ± 0,005	–	0,00747 ± 0,00023
Mn	0,666 ± 0,010	0,743 ± 0,013	0,769 ± 0,008	0,289 ± 0,004	0,2160 ± 0,0014
P	0,0057R ± 0,0004	0,0234 ± 0,0012	0,013 ± 0,001	0,0076 ± 0,0010	0,0106 ± 0,0003
S	0,024 ± 0,024	0,192 ± 0,006	0,030 ± 0,001	0,0100 ± 0,0005	0,00561 ± 0,00021
Cr	0,016 ± 0,004	0,0382 ± 0,0023	0,018 ± 0,001	(0,0129)	0,0219 ± 0,0003
Mo	–	–	–	–	–
Ni	0,029 ± 0,002	0,0219 ± 0,0010	0,027 ± 0,001	0,014 ± 0,001	0,0116 ± 0,0003
Al	0,010 ± 0,001	0,0209 ± 0,0017	0,032 ± 0,002	(0,0044)	0,0784 ± 0,0012
As	–	0,0040 ± 0,0007	(0,029)	(0,0043)	0,00177 ± 0,00009
Co					0,00236 ± 0,00009
Cu	0,041 ± 0,002	0,0462 ± 0,0010	0,025 ± 0,001	0,016 ± 0,001	0,0127 ± 0,0002
N	0,0078 ± 0,0007	0,0074 ± 0,0005	0,0046 ± 0,0004	0,00189 ± 0,00011	0,00157 ± 0,00010
Nb	0,054 ± 0,005	–	–	–	–
Pb	–	–	0,149 ± 0,004	–	–
Sn	–	0,0037 ± 0,0008	–	–	–
Ti	–	(0,0021)	–	–	–
V	–	–	–	–	–
Te	–	–	0,030 ± 0,001	–	–
Zn	–	–	–	–	0,00439 ± 0,00015

CRM-No.	D 049-1	D 077-3
Year of issue	2020	2017
Chips, powder	•	•
C	0,701 ± 0,004 ⁺	0,1650 ± 0,0016 ⁺
S	0,00404 ± 0,00017 ⁺	0,0162 ± 0,0003
N	0,00317 ± 0,00015 ⁺	1,274 ± 0,014

(Values in parentheses are indicative values)

R: revised value

⁺ 95%-confidence interval

Pure iron

Disc

Mass fraction in µg/g
± 95%-confidence interval

CRM-No.	D 098-1
Year of issue	1993
C	5,1 ± 1,3
Si	4,8 ± 1,1
Mn	0,8 ± 0,4
P	(0,6)
S	3,1 ± 0,5
Cr	57,1 ± 2,4
Mo	8,5 ± 0,8
N	2,4 ± 0,7

(Values in parentheses are indicative values)

Alloy steels

Mass fraction in % ± standard deviation

CRM-No.	D 126-1	D 128-1	D 129-3	D 130-1
Year of issue	1963	1972	2008	1968
Chips, powder	•	•	•	•
Disc			•	
C	0,841 ± 0,008	0,085 ± 0,003	0,3684 ± 0,0017 ⁺	0,546 ± 0,005
Si	(0,241)	0,949 ± 0,010	0,2087 ± 0,0020 ⁺	0,313 ± 0,006
Mn	1,817 ± 0,009	0,839 ± 0,010	0,371 ± 0,004 ⁺	1,593 ± 0,009
P	0,0092 ± 0,0011	0,007 ± 0,001	0,0110 ± 0,0003 ⁺	0,0209 ± 0,0017
S	0,0050 ± 0,0007	0,007 ± 0,001	0,0165 ± 0,0003 ⁺	0,0158 ± 0,0011
Cr	0,317 ± 0,009	0,108 ± 0,003	1,702 ± 0,008 ⁺	(0,032)
Mo	–	–	0,206 ± 0,003 ⁺	–
Ni	(0,038)	0,046 ± 0,006	1,022 ± 0,007 ⁺	(0,031)
Al	–	0,286 ± 0,010	1,016 ± 0,006 ⁺	0,0037 ± 0,0005
Al _{acid soluble}	–	–	–	0,0019 ± 0,0006
As	–	–	0,0049 ± 0,0003 ⁺	0,0167 ± 0,0011
B	–	–	(0,0012)	–
Co	–	–	0,0148 ± 0,0002 ⁺	–
Cu	(0,098)	0,055 ± 0,003	0,0804 ± 0,0007 ⁺	0,072 ± 0,003
N	–	(0,0024)	0,0046 ± 0,0002 ⁺	0,0093 ± 0,0008
Nb	–	–	(0,0007)	–
Pb	–	–	–	–
Sn	–	–	0,0067 ± 0,0002 ⁺	(0,006)
Ti	–	0,890 ± 0,013	0,0030 ± 0,0002 ⁺	–
V	0,143 ± 0,004	(0,008)	(0,0045)	(0,003)
W	–	–	(0,0052)	–
Bi	–	–	–	–
Ca	–	–	–	–
Cd	–	–	–	–
Ga	–	–	–	–
Hg	–	–	–	–
Mg	–	–	–	–
Sb	–	–	0,00059 ± 0,00008 ⁺	–
Se	–	–	–	–
Te	(0,0002)	–	–	–
Tl	–	–	–	–
Zn	–	–	(0,0030)	–

(Values in parentheses are indicative values)

⁺ 95%-confidence interval

R: revised value

- continued -

Alloy steels (continued)

CRM-No.	D 179-2	D 180-1	D 182-1	D 183-1
Year of issue	1990	1973	1974	1973
Chips, powder	•	•	•	•
Disc	•			
C	0,598 ± 0,009	0,197 ± 0,005	0,790 ± 0,008	0,083 ± 0,002
Si	0,579 ± 0,011	0,362 ± 0,007	0,368 ± 0,014	0,421 ± 0,006
Mn	0,539 ± 0,010	1,286 ± 0,015	0,389 ± 0,007	0,354 ± 0,004
P	0,0267 ± 0,0024	0,0174 ± 0,0010	0,0076R± 0,0005	0,089 ± 0,002
S	(0,0006)	0,0249 ± 0,0010	0,011 ± 0,001	0,031 ± 0,001
Cr	1,08 ± 0,03	1,250 ± 0,018	0,591 ± 0,012	0,670 ± 0,013
Mo	0,070± 0,006	–	–	–
Ni	0,0741R± 0,0008	0,096 ± 0,008	0,152 ± 0,005	0,073 ± 0,004
Al	–	–	0,020 ± 0,003	0,027 ± 0,002
Al _{acid soluble}	–	–	–	–
As	–	0,030 ± 0,002	(0,0202)	(0,013)
B	–	–	–	–
Co	(0,015)	–	–	–
Cu	0,111 ± 0,004	0,115 ± 0,004	0,141 ± 0,004	0,445 ± 0,010
N	0,0068 ± 0,0003 ⁺	0,0068 ± 0,0009	0,0102 ± 0,0004	0,0064 ± 0,0006
Nb	0,00144± 0,00013 ⁺	–	–	–
Pb	0,00013± 0,00002 ⁺	–	0,0039 ± 0,0003	–
Sn	–	–	(0,0135)	–
Ti	(0,0014)	–	–	–
V	0,188± 0,007	–	0,177 ± 0,010	–
W	1,87± 0,05	–	–	–
Bi	< 0,00003	–	–	–
Ca	–	–	–	–
Cd	< 0,00003	–	–	–
Ga	0,00129± 0,00012 ⁺	–	–	–
Hg	(< 0,00001)	–	–	–
Mg	–	–	(0,0005)	–
Sb	0,00175± 0,00010 ⁺	–	0,0042 ± 0,0005	–
Se	(< 0,00020)	–	–	–
Te	< 0,00020	–	–	–
Tl	(< 0,000035)	–	–	–
Zn	0,00023± 0,00004 ⁺	–	0,0015 ± 0,0002	–

(Values in parentheses are indicative values)

R: revised value

- continued -

Alloy steels (continued)

CRM-No.	D 187-1	D 187-2	D 191-2	D 191-3
Year of issue	1982	2010	2006	2021
Chips,powder	•	•	•	•
Disc		•		•
C	0,195 ± 0,003	0,2038 ± 0,0012	0,0043 ± 0,0002 ⁺	0,0027 ± 0,0002 ⁺
Si	0,026 ± 0,002	0,2110 ± 0,0029	3,267 ± 0,012 ⁺	3,226 ± 0,020 ⁺
Mn	1,354 ± 0,011	1,257 ± 0,006	0,1334 ± 0,0019 ⁺	0,1539 ± 0,0015 ⁺
P	0,014 ± 0,001	0,0066 ± 0,0002	0,0087 ± 0,0004 ⁺	0,0097 ± 0,0004 ⁺
S	0,025 ± 0,001	0,0300 ± 0,0006	0,0029 ± 0,0002 ⁺	0,0005 ± 0,0001 ⁺
Cr	1,186 ± 0,015	1,132 ± 0,007	0,0314 ± 0,0006 ⁺	0,0242 ± 0,0005 ⁺
Mo	0,035 ± 0,002	0,0623 ± 0,0008	0,0020 ± 0,0002 ⁺	0,00127 ± 0,00008 ⁺
Ni	0,096 ± 0,003	0,1755 ± 0,0013	0,0224 ± 0,0004 ⁺	0,0124 ± 0,0003 ⁺
Al	0,046 ± 0,002	0,0223 ± 0,0006	0,985 ± 0,006 ⁺	0,815 ± 0,011 ⁺
Al_{acid soluble}	–	–	–	–
As	0,018 ± 0,002	0,0057 ± 0,0003	0,0018 ± 0,0003 ⁺	0,00144 ± 0,00012 ⁺
B	0,0004 ± 0,0002	0,00048 ± 0,00006	–	0,00024 ± 0,00006 ⁺
Co	0,014 ± 0,001	0,0112 ± 0,0003	–	(0,0017)
Cu	0,161 ± 0,003	0,1288 ± 0,0012	0,0165 ± 0,0003 ⁺	0,0097 ± 0,0002 ⁺
N	0,014 ± 0,001	0,0105 ± 0,0004	0,00105 ± 0,00009 ⁺	0,00105 ± 0,00010 ⁺
Nb	–	–	–	(0,00008)
Pb	–	–	–	(0,0002)
Sn	0,011 ± 0,001	0,0237 ± 0,0006	0,0050 ± 0,0005 ⁺	0,00131 ± 0,00011 ⁺
Ti	–	(0,00075)	0,0024 ± 0,0002 ⁺	0,0020 ± 0,0001 ⁺
V	–	0,0122 ± 0,0003	–	0,00043 ± 0,00004 ⁺
W	–	–	–	(0,0001)
Ca	–	–	–	(0,0007)
Mg	–	–	–	0,0036 ± 0,0002 ⁺
Sb	–	(0,0018)	(0,0007)	(0,0004)
Te	–	–	–	–
Zn	–	–	–	(0,0009)

(Values in parentheses are indicative values)

R: revised value ⁺ 95%-confidence interval

Alloy steels (continued)

CRM-No.	D 192-1	D 193-1	D 194-1	D 194-2
Year of issue	1994	1990	1993	2015
Chips,powder	•	•	•	•
Disc	•	•		
C	0,1875 ± 0,0009	0,139 ± 0,004	0,1532 ± 0,0011 ⁺	0,1694 ± 0,0010 ⁺
Si	0,219 ± 0,004	0,404 ± 0,006	0,431 ± 0,004 ⁺	0,2974 ± 0,0029 ⁺
Mn	1,377 ± 0,006	0,972 ± 0,017	1,188 ± 0,004 ⁺	1,282 ± 0,009 ⁺
P	0,0029 ± 0,0002	0,0063 ± 0,0006	0,0097 ± 0,0006 ⁺	0,0137 ± 0,0003 ⁺
S	0,0010 ± 0,0001	0,0086 ± 0,0006	0,000059R ± 0,00005 ⁺	0,00049 ± 0,00009 ⁺
Cr	0,0717 ± 0,0018	0,182 ± 0,006	0,733 ± 0,006 ⁺	0,760 ± 0,006 ⁺
Mo	0,482 ± 0,004	0,347 ± 0,011	0,2857 ± 0,0026 ⁺	0,402 ± 0,004 ⁺
Ni	0,755 ± 0,004	1,178 ± 0,019	0,3417 ± 0,0027 ⁺	0,3316 ± 0,0023 ⁺
Al	0,0308 ± 0,0008	0,0257 ± 0,0015	0,0837 ± 0,0020 ⁺	0,0669 ± 0,0009 ⁺
Al _{acid soluble}	0,0285 ± 0,0008	—	—	—
As	(0,003)	0,0062 ± 0,0007	0,0042 ± 0,0004 ⁺	0,00208 ± 0,00011 ⁺
B	(0,00016)	(0,0002)	0,0020 ± 0,0002 ⁺	0,00155 ± 0,00016 ⁺
Co	0,0055 ± 0,0002	0,0073 ± 0,0007	—	0,00328 ± 0,00011 ⁺
Cu	0,0453 ± 0,0008	0,598 ± 0,009	0,0751 ± 0,0011 ⁺	0,0313 ± 0,0004 ⁺
N	0,0118 ± 0,0002	0,0108 ± 0,0004	0,0115 ± 0,0002 ⁺	0,00319 ± 0,00014 ⁺
Nb	—	0,0232 ± 0,0019	—	0,0290 ± 0,0007 ⁺
Pb	—	(0,0002)	—	—
Sn	(0,0030)	—	—	(0,00036)
Ti	(0,0009)	(0,0013)	—	0,00322 ± 0,00015 ⁺
V	(0,003)	(0,0019)	0,0243 ± 0,0009 ⁺	0,00161 ± 0,00010 ⁺
W	—	—	—	—
Ca	—	—	0,0026 ± 0,0002 ⁺	—
Mg	—	—	—	—
Sb	—	—	—	(0,00030)
Te	—	—	—	—
Zn	—	—	—	—

(Values in parentheses are indicative values)

R: revised value

⁺ 95%-confidence interval

Highly alloyed steels

Mass fraction in % $\pm$ standard deviation

CRM-No.	D 227-1	D 231-2	D 235-1	D 237-1
Year of issue	1971	2002	1972	1973
Chips	•	•	•	•
Disc				
C	0,950 $\pm$ 0,013	0,0140 $\pm$ 0,0003 ⁺	0,912 $\pm$ 0,014	0,068 $\pm$ 0,002
Si	0,272 $\pm$ 0,013	0,368 $\pm$ 0,006 ⁺	0,094 $\pm$ 0,010	0,482 $\pm$ 0,013
Mn	0,236 $\pm$ 0,007	1,263 $\pm$ 0,009 ⁺	12,73 $\pm$ 0,07	1,443 $\pm$ 0,018
P	0,016 $\pm$ 0,001	0,0179 $\pm$ 0,0007 ⁺	0,045 $\pm$ 0,002	0,032 $\pm$ 0,002
S	0,022 $\pm$ 0,002	0,0250 $\pm$ 0,0007 ⁺	0,0072 $\pm$ 0,0007	0,012 $\pm$ 0,001
Cr	4,25 $\pm$ 0,02	18,071 $\pm$ 0,018 ⁺	0,354 $\pm$ 0,014	17,24 $\pm$ 0,04
Mo	2,64 $\pm$ 0,05	0,301 $\pm$ 0,004 ⁺	0,032 $\pm$ 0,003	0,306 $\pm$ 0,006
Ni	0,114 $\pm$ 0,008	10,105 $\pm$ 0,021 ⁺	(0,08)	10,32 $\pm$ 0,04
Al	–	0,0032 $\pm$ 0,0004 ⁺	–	–
As	–	0,0048 $\pm$ 0,0003 ⁺	–	–
B	–	0,0020 $\pm$ 0,0002 ⁺	–	–
Co	–	0,0402 $\pm$ 0,0011 ⁺	–	0,221 $\pm$ 0,006
Cu	0,124 $\pm$ 0,005	0,0941 $\pm$ 0,0009 ⁺	0,073 $\pm$ 0,002	0,123 $\pm$ 0,005
N	0,040 $\pm$ 0,002	0,0444 $\pm$ 0,0004 ⁺	0,020 $\pm$ 0,0008	0,035 $\pm$ 0,002
Nb	–	–	–	0,660 $\pm$ 0,023
Pb	–	(0,00007)	–	–
Sn	0,0251 $\pm$ 0,0024	0,0043 $\pm$ 0,0003 ⁺	–	–
Ti	–	0,0007 $\pm$ 0,0002 ⁺	–	–
V	2,44 $\pm$ 0,03	0,0708 $\pm$ 0,0008 ⁺	(0,012)	0,057 $\pm$ 0,005
W	3,03 $\pm$ 0,06	0,0141 $\pm$ 0,0010 ⁺	–	–
Zr	–	–	–	–
Ag	(0,000064)	–	–	–
O	–	–	–	–
Sb	0,0035 $\pm$ 0,0005	0,0011 $\pm$ 0,0001 ⁺	–	–
Ta	–	–	–	–
Ca	–	0,00074 $\pm$ 0,00014 ⁺	–	–

(Values in parentheses are indicative values)

⁺95%-confidence interval

- continued -

Highly alloyed steels (continued)

CRM-No.	D 271-1	D 278-1	D 283-1	D 284-2	D 284-3
Year of issue	2007	1973	1985	2000	2016
Chips	•	•	•	•	•
Disc	•				•
C	0,3698 ± 0,0021 ⁺	0,903 ± 0,019	1,219 ± 0,009	0,0201 ± 0,0005 ⁺	0,0025 ± 0,0003 ⁺
Si	0,923 ± 0,006 ⁺	0,336 ± 0,008	0,345 ± 0,017	0,537 ± 0,008 ⁺	0,0442 ± 0,0017 ⁺
Mn	0,437 ± 0,004 ⁺	0,405 ± 0,006	0,217 ± 0,010	1,745 ± 0,009 ⁺	0,0615 ± 0,0012 ⁺
P	0,0120 ± 0,0004 ⁺	0,0154 ± 0,0014	0,022 ± 0,002	0,0258 ± 0,0008 ⁺	0,0049 ± 0,0003 ⁺
S	0,00045 ± 0,00008 ⁺	0,0052 ± 0,0011	0,029 ± 0,002	0,0237 ± 0,0005 ⁺	0,0066 ± 0,0003 ⁺
Cr	5,002 ± 0,019 ⁺	18,11 ± 0,08	4,15 ± 0,06	16,811 ± 0,019 ⁺	17,37 ± 0,04 ⁺
Mo	1,247 ± 0,006 ⁺	1,040 ± 0,030	3,41 ± 0,09	2,111 ± 0,010 ⁺	2,236 ± 0,012 ⁺
Ni	0,1552 ± 0,0020 ⁺	0,236 ± 0,024	–	10,72 ± 0,05 ⁺	12,09 ± 0,04 ⁺
Al	0,0234 ± 0,0011 ⁺	–	0,0099 ± 0,0014	0,0027 ± 0,0004 ⁺	(0,0471)
As	0,0057 ± 0,0004 ⁺	–	(0,0096)	0,0063 ± 0,0003 ⁺	0,00131 ± 0,00011 ⁺
B	(0,0003)	–	0,0003 ± 0,0001	0,0026 ± 0,0001 ⁺	0,00020 ± 0,00004 ⁺
Co	0,0139 ± 0,0005 ⁺	–	10,27 ± 0,17	0,0525 ± 0,0011 ⁺	0,0366 ± 0,0007 ⁺
Cu	0,1371 ± 0,0015 ⁺	0,077 ± 0,008	–	0,1831 ± 0,0014 ⁺	0,0105 ± 0,0004 ⁺
N	0,0137 ± 0,0003 ⁺	–	0,033 ± 0,002	0,0151 ± 0,0002 ⁺	0,0418 ± 0,0008 ⁺
Nb	(0,0009)	–	–	(0,0028)	(0,0129)
Pb	(0,0005)	–	(< 0,0005)	–	(0,0003)
Sn	0,0084 ± 0,0002 ⁺	–	(0,0065)	0,0047 ± 0,0002 ⁺	0,00074 ± 0,00009 ⁺
Ti	0,0020 ± 0,0002 ⁺	–	–	0,191 ± 0,004 ⁺	0,0050 ± 0,0004 ⁺
V	0,850 ± 0,007 ⁺	0,077 ± 0,008	3,28 ± 0,03	0,0425 ± 0,0016 ⁺	(0,0947)
W	0,0054 ± 0,0005 ⁺	–	9,66 ± 0,12	(0,0183)	0,0039 ± 0,0003 ⁺
Zr	(0,00013)	–	–	(0,0005)	(0,00353)
Ag	–	–	–	–	–
Ca	0,0009 ± 0,0002 ⁺	–	–	–	–
Mg	(0,00013)	–	–	–	–
O	0,0020 ± 0,0002 ⁺¹⁾	–	–	0,0099 ± 0,0007 ⁺²⁾	–
Sb	(0,0017)	–	–	–	(0,000365)
Ta	–	–	–	(0,0013)	–
Ga	–	–	–	–	(0,0016)
Ir	–	–	–	–	(0,000005)
Re	–	–	–	–	(0,0005)

(Values in parentheses are indicative values)

¹⁾ Oxygen certified only for disc

²⁾ Oxygen certified only for chips

⁺95%-confidence interval
– continued–

Highly alloyed steels (continued)

CRM-No.	D 286-2	D 288-1	D 289-1	D 290-1 ¹⁾	D 291-1 ¹⁾
Year of issue	2023	1986	1990	1990	1990
Chips	•	•	•	•	•
Disc		•	•	•	•
C	0,0640 ± 0,0012 ⁺	2,08 ± 0,02	0,0489 ± 0,0022	0,911 ± 0,010	0,903 ± 0,008
Si	0,394 ± 0,007 ⁺	0,260 ± 0,012	0,531 ± 0,013	0,072 ± 0,007	0,907 ± 0,018
Mn	1,919 ± 0,011 ⁺	0,292 ± 0,008	1,016 ± 0,016	0,244 ± 0,010	0,808 ± 0,011
P	0,0306 ± 0,0009 ⁺	0,024 ± 0,002	0,0114 ± 0,0010	0,0160 ± 0,0005	0,0168 ± 0,0016
S	0,305 ± 0,004 ⁺	(0,0012)	0,0027 ± 0,0004	0,0160 ± 0,0008	0,0087 ± 0,0007
Cr	17,65 ± 0,06 ⁺	12,00 ± 0,08	14,63 ± 0,11	4,18 ± 0,06	17,10 ± 0,10
Mo	0,413 ± 0,005 ⁺	0,103 ± 0,007	1,102 ± 0,015	4,83 ± 0,09	2,10 ± 0,06
Ni	8,436 ± 0,030 ⁺	0,298 ± 0,007	24,68 ± 0,19	0,329 ± 0,018	0,563 ± 0,011
Al	(0,0019)	0,012 ± 0,002	0,199 ± 0,011	–	0,0030 ± 0,0006
As	–	(0,0065)	(0,0056)	–	–
B	–	–	0,0044 ± 0,0004	–	–
Co	0,1490 ± 0,0017 ⁺	0,018 ± 0,002	0,065 ± 0,006	5,12 ± 0,12	0,0233 ± 0,0022
Cu	0,370 ± 0,004 ⁺	0,060 ± 0,004	–	0,081 ± 0,004	0,0711 ± 0,0019
N	0,0350 ± 0,0009 ⁺	0,0151 ± 0,0004	–	0,0325 ± 0,0012	0,1142 ± 0,0038
Nb	(0,011)	–	–	–	(0,0057)
Pb	(0,00021)	–	(0,0008)	–	–
Sn	0,0097 ± 0,0004 ⁺	(0,0043)	0,111 ± 0,010	–	–
Ti	(0,0005)	0,020 ± 0,002	2,01 ± 0,05	–	–
V	–	0,055 ± 0,004	0,260 ± 0,015	1,91 ± 0,04	0,388 ± 0,016
W	(0,0383)	(0,682)	–	6,27 ± 0,14	–
Zr	–	–	–	–	–
Ag	–	–	–	–	–
Ca	–	–	–	–	–
O	–	–	–	–	–
Sb	–	(0,0014)	(0,0013)	–	–
Ta	–	–	–	–	–
Te	–	–	–	–	–

(Values in parentheses are indicative values)

⁺95%-confidence interval

- continued-

¹⁾ Powdered material, produced by atomization of the melt

Highly alloyed steels (continued)

CRM-No.	D 294-1	D 297-1	D 299-1
Year of issue	2005	2005	2009
Chips	•	•	•
Disc	•	•	
C	0,0657 ± 0,0010 ⁺	0,0223 ± 0,0004 ⁺	0,0154 ± 0,0006 ⁺
Si	0,283 ± 0,005 ⁺	0,344 ± 0,006 ⁺	0,299 ± 0,005 ⁺
Mn	18,68 ± 0,04 ⁺	0,897 ± 0,007 ⁺	0,2678 ± 0,0026 ⁺
P	0,0273 ± 0,0013 ⁺	0,0135 ± 0,0004 ⁺	0,0152 ± 0,0006 ⁺
S	0,00031 ± 0,00009 ⁺	0,0101 ± 0,0003 ⁺	0,00022 ± 0,00006 ⁺
Cr	17,98 ± 0,05 ⁺	18,37 ± 0,03 ⁺	22,32 ± 0,05 ⁺
Mo	0,0861 ± 0,0022 ⁺	0,290 ± 0,005 ⁺	0,0186 ± 0,0010 ⁺
Ni	0,427 ± 0,006 ⁺	12,33 ± 0,02 ⁺	0,172 ± 0,004 ⁺
Al	(0,0095)	0,0195 ± 0,0009 ⁺	5,33 ± 0,04 ⁺
As	0,00365 ± 0,00029 ⁺	0,0040 ± 0,0005 ⁺	0,0054 ± 0,0004 ⁺
B	(<0,00005)	1,146 ¹⁾ ± 0,009 ⁺	0,0002 ± 0,0001 ⁺
Co	0,0288 ± 0,0009	0,0413 ± 0,0007 ⁺	0,0187 ± 0,0010 ⁺
Cu	0,0242 ± 0,0007 ⁺	0,204 ± 0,004 ⁺	0,0382 ± 0,0008 ⁺
N	0,566 ± 0,011 ⁺	0,0152 ± 0,0007 ⁺	0,0198 ± 0,0008 ⁺
Nb	(0,00117)	(0,0089)	(0,0043)
Pb	(0,000128)	–	(0,0018)
Sn	(0,0014)	–	(0,0079)
Ti	(0,0008)	0,0072 ± 0,0004 ⁺	0,1289 ± 0,0018 ⁺
V	0,0694 ± 0,0021 ⁺	0,0535 ± 0,0008 ⁺	0,0333 ± 0,0015 ⁺
W	(0,00114)	(0,0057)	(0,0017)
Zr	(0,0001)	(0,0002)	0,1775 ± 0,0025 ⁺
Ag	–	–	–
Ca	(0,00026)	(0,0002)	–
O	–	–	–
Sb	(0,00053)	–	(0,0005)
Ta	–	–	–
Te	(<0,00008)	–	–

(Values in parentheses are indicative values)

*95%-confidence interval

¹⁾ Boron isotope ratio ¹⁰B/¹¹B (0,24811)

Special alloys

Chips

Mass fraction in % $\pm$ standard deviation

CRM-No.	D 326-1	D 327-2	D 328-1
Year of issue	1972	1972	1973
C	0,092 $\pm$ 0,002	0,152 $\pm$ 0,003	0,390 $\pm$ 0,005
Si	1,46 $\pm$ 0,025	2,052 $\pm$ 0,028	0,629 $\pm$ 0,014
Mn	0,406 $\pm$ 0,008	1,289 $\pm$ 0,018	1,395 $\pm$ 0,012
P	0,0093 $\pm$ 0,0009	0,0228 $\pm$ 0,0014	0,005 $\pm$ 0,001
S	0,0028 $\pm$ 0,0006	0,0046 $\pm$ 0,0012	0,003 $\pm$ 0,001
Cr	16,37 $\pm$ 0,05	24,35 $\pm$ 0,08	20,54 $\pm$ 0,07
Mo	(0,025)	0,174 $\pm$ 0,009	4,41 $\pm$ 0,07
Ni	61,16 $\pm$ 0,16	19,72 $\pm$ 0,08	20,38 $\pm$ 0,19
Al _{total}	(0,79)	0,070 $\pm$ 0,006	0,070 $\pm$ 0,006
Co	0,223 $\pm$ 0,011	0,159 $\pm$ 0,010	41,65 $\pm$ 0,24
Cu	(0,027)	0,060 $\pm$ 0,003	0,013 $\pm$ 0,003
N	(0,0359)	0,059 $\pm$ 0,0024	0,027 $\pm$ 0,002
Nb	–	–	3,61 $\pm$ 0,22
V	(0,024)	0,044 $\pm$ 0,004	–
W	–	–	4,16 $\pm$ 0,04
Zr	0,129 $\pm$ 0,008	–	–
Fe	–	–	2,40 $\pm$ 0,06
Ta	–	–	0,18 $\pm$ 0,02

(Values in parentheses are indicative values)

Cast irons

Mass fraction in % ± standard deviation

CRM-No.	D 428-2 ¹⁾	D 476-3	D 478-2	D 480-1 ¹⁾
Year of issue	1998	1996	1996	1979
Chips, powder	•	•	•	•
Disc				
C_{total}	2,747 ± 0,009 ⁺	3,390 ± 0,011 ⁺	4,003 ± 0,013 ⁺	3,03 ± 0,02
Si	1,752 ± 0,007 ⁺	1,813 ± 0,005 ⁺	2,411 ± 0,021 ⁺	2,41 ± 0,02
Mn	0,750 ± 0,05 ⁺	0,987 ± 0,008 ⁺	0,321 ± 0,005 ⁺	0,151 ± 0,005
P	0,0691 ± 0,0011 ⁺	0,0908 ± 0,0023 ⁺	0,201 ± 0,006 ⁺	0,0021 R ± 0,0005
S	0,1105 ± 0,0018 ⁺	0,0493 ± 0,0009 ⁺	0,0460 ± 0,0015 ⁺	0,0086 ± 0,0010
Cr	0,0366 ± 0,0017 ⁺	0,0648 ± 0,0012 ⁺	0,251 ± 0,005 ⁺	(0,0164)
Mo	(0,0014)	–	–	–
Ni	0,0358 ± 0,0005 ⁺	0,0549 ± 0,0014 ⁺	0,151 ± 0,007 ⁺	0,483 ± 0,007
Al	–	–	–	0,016 ± 0,001
As	0,0156 ± 0,0005 ⁺	0,0145 ± 0,0007 ⁺	(0,0018)	–
B	–	–	0,0006 ± 0,0001 ⁺	–
Cu	0,0996 ± 0,0014 ⁺	0,2445 ± 0,0025 ⁺	0,1276 ± 0,0019 ⁺	(0,0052)
N	–	0,0038 ± 0,0001 ⁺	0,0023 ± 0,0002 ⁺	–
Ti	0,0311 ± 0,0005 ⁺	0,0222 ± 0,0005 ⁺	0,0328 ± 0,0007 ⁺	–
V	0,0120 ± 0,0003 ⁺	0,0115 ± 0,0002 ⁺	0,0113 ± 0,0003 ⁺	–
Mg	–	–	–	0,017 ± 0,001

(Values in parentheses are indicative values)

R: revised value

⁺ 95%-confidence interval

¹⁾ Powdered material, produced by atomization of the melt

Ferro alloys

Powder

Mass fraction in % $\pm$ 95% confidence interval

CRM-No.	D 502-2	D 529-1	D 578-2	D 589-2	D 591-2	D 593-1
Description	FeMn	FeSi	FeMo	FeTi	FeV	FeV
Year of issue	2004	1975	2023	2023	2022	2022
C	6,94 $\pm$ 0,02	0,10 $\pm$ 0,01 ⁺	0,0200 $\pm$ 0,0014*	0,179 $\pm$ 0,005*	0,0206 $\pm$ 0,0014	0,555 $\pm$ 0,006
Si	(0,092)	91,11 $\pm$ 0,33 ⁺	(0,1845)	(0,3516)	0,246 $\pm$ 0,013	4,73 $\pm$ 0,05
Mn	77,87 $\pm$ 0,11	0,04 $\pm$ 0,005 ⁺	(0,0075)	0,247 $\pm$ 0,005*	0,0207 $\pm$ 0,0007 ⁺	0,861 $\pm$ 0,010
P	0,148 $\pm$ 0,003	0,013 $\pm$ 0,001 ⁺	0,0221 $\pm$ 0,0007*	–	0,0050 $\pm$ 0,0003	0,116 $\pm$ 0,004
S	(0,0024)	–	0,0311 $\pm$ 0,0010*	0,0101 $\pm$ 0,0006*	0,0037 $\pm$ 0,0004	0,198 $\pm$ 0,004
Cr	0,0265 $\pm$ 0,0006	–	(0,0117)	(1,060)	(0,0342)	0,621 $\pm$ 0,015
Mo	–	–	72,19 $\pm$ 0,18*	0,549 $\pm$ 0,014*	(0,0318)	0,422 $\pm$ 0,009
Ni	0,0384 $\pm$ 0,0011	–	0,0299 $\pm$ 0,0007*	0,191 $\pm$ 0,005*	0,0086 $\pm$ 0,0005	0,451 $\pm$ 0,006
Al	–	0,86 $\pm$ 0,02 ⁺	–	3,172 $\pm$ 0,023*	(0,979)	(0,027)
Al_{sol}	–	–	–	–	(0,652)	(0,022)
As	–	–	–	–	0,0045 $\pm$ 0,0002	0,0028 $\pm$ 0,0003
B	(0,0006)	–	–	–	0,00046 $\pm$ 0,00008	0,0052 $\pm$ 0,0004
Co	(0,048)	–	0,0069 $\pm$ 0,0004*	0,0149 $\pm$ 0,0006*	(0,0023)	(0,0046)
Cu	0,0370 $\pm$ 0,0007	0,01 $\pm$ 0,001 ⁺	0,3497 $\pm$ 0,0029*	0,0697 $\pm$ 0,0018*	0,0036 $\pm$ 0,0002	0,116 $\pm$ 0,003
N	(0,017)	–	–	–	(0,040)	(0,48)
Sn	–	–	0,00305 $\pm$ 0,00012*	0,167 $\pm$ 0,006*	(0,00076)	0,0048 $\pm$ 0,0003
Sb	–	–	0,0018 $\pm$ 0,0004*	–	–	–
Ti	0,0034 $\pm$ 0,0003	0,09 $\pm$ 0,004 ⁺	–	68,94 $\pm$ 0,23*	0,0017 $\pm$ 0,0002	0,0147 $\pm$ 0,0005
V	–	–	–	(1,336)	84,28 $\pm$ 0,10	67,05 $\pm$ 0,06
W	–	–	–	–	(0,0018)	(0,0046)
Zr	–	–	–	0,260 $\pm$ 0,007*	–	–
Ca	–	0,46 $\pm$ 0,04 ⁺	–	(0,0404)	–	–
Fe	(14,6)	6,15 $\pm$ 0,08 ⁺	(27,3)	(22,0)	13,86 $\pm$ 0,07	(23,6)
Mg	–	0,04 $\pm$ 0,006 ⁺	–	(0,101)	–	(0,0232)
O	–	–	–	–	–	–
Bi	–	–	(0,00011)	–	–	–
Zn	–	–	–	(0,0113)	0,0181 $\pm$ 0,0008	0,0088 $\pm$ 0,0005
Pb	0,0179 $\pm$ 0,0011	–	(0,00051)	(0,0061)	(0,00029)	(0,0020)

(Values in parentheses are indicative values)

* standard deviation

* estimated expanded uncertainty

Ores, iron oxide

Powder

Mass fraction in % $\pm$ standard deviation

CRM-No.	D 630-1	D 631-1	D 633-1
Description	Iron ore	Iron ore	Manganese ore
Year of issue	1969	1969	1967
Fe_{total}	65,63 $\pm$ 0,17	61,09 $\pm$ 0,09	1,64 $\pm$ 0,04
Si	–	–	–
SiO ₂	5,88 $\pm$ 0,07	3,20 $\pm$ 0,06	10,39 $\pm$ 0,15
Al	–	–	–
Al ₂ O ₃	0,88 $\pm$ 0,038	1,06 $\pm$ 0,05	1,64 $\pm$ 0,12
Ca	–	–	–
CaO	0,10 $\pm$ 0,017	0,75 $\pm$ 0,038	2,02 $\pm$ 0,12
Mg	–	–	–
MgO	0,47 $\pm$ 0,046	0,54 $\pm$ 0,059	0,58 $\pm$ 0,10
Mn	0,060 $\pm$ 0,005	0,044 $\pm$ 0,006	47,85 $\pm$ 0,21
P	0,043 $\pm$ 0,003	0,114 $\pm$ 0,005	0,170 $\pm$ 0,007
S	0,032 $\pm$ 0,004	0,033 $\pm$ 0,006	0,227 $\pm$ 0,009
Na	–	–	–
Na ₂ O	–	(0,04)	–
K	–	–	–
K ₂ O	–	(0,04)	–
As	–	–	(0,0040)
BaO	–	–	1,13 $\pm$ 0,08
Cr	–	–	–
Cu	–	–	–
F	–	–	–
Ni	–	–	–
Pb	–	–	–
Ti	–	–	–
TiO ₂	0,066 $\pm$ 0,013	0,109 $\pm$ 0,006	0,079 $\pm$ 0,009
V	–	–	–
Zn	–	–	–

(Values in parentheses are indicative values)

- continued-

Ores, iron oxide (continued)

CRM-No.	D 680-1		D 686-1		D 687-1	
Description	Iron ore		Iron oxide		Iron oxide	
Year of issue	1977		2002		2009	
Fe total	59,98	± 0,08	69,44	± 0,11 ⁺	69,66	± 0,14 ⁺
Fe(II)	—		(0,0484)		(0,076)	
Si	4,20	± 0,02	0,0083	± 0,0005 ⁺	0,0157	± 0,0011 ⁺
SiO₂	8,98	± 0,04	—		—	
Al	0,66	± 0,02	0,0407	± 0,0012 ⁺	0,0356	± 0,0012 ⁺
Al₂O₃	1,23	± 0,04	—		—	
Ca	0,45	± 0,02	0,0097	± 0,0007 ⁺	0,0113	± 0,0012 ⁺
CaO	0,63	± 0,03	—		—	
Mg	0,14	± 0,01	0,0027	± 0,0002 ⁺	0,0018	± 0,0002 ⁺
MgO	0,23	± 0,02	—		—	
Mn	0,025	± 0,002	0,231	± 0,004 ⁺	0,1658	± 0,0027 ⁺
P	0,018	± 0,002	0,0078	± 0,0001 ⁺	0,0120	± 0,0004 ⁺
P₂O₅	—		—		—	
S	0,544	± 0,017	—		—	
Na	0,128	± 0,004	0,0058	± 0,0005 ⁺	0,0030	± 0,0003 ⁺
Na₂O	—		—		—	
K	0,078	± 0,003	0,0024	± 0,0004 ⁺	0,0011	± 0,0002 ⁺
K₂O	—		—		—	
As	0,057	± 0,003	—		—	
Cr	0,005	± 0,001	0,0182	± 0,0006 ⁺	0,0227	± 0,0008 ⁺
Cu	0,063	± 0,003	0,0038	± 0,0003 ⁺	0,0030	± 0,0003 ⁺
F	—		—		—	
Ni	0,007	± 0,001	0,0127	± 0,0004 ⁺	0,0122	± 0,0006 ⁺
Pb	0,317	± 0,008	—		(0,0004)	
Ti	0,045	± 0,003	0,0014	± 0,0001 ⁺	0,0303	± 0,0005 ⁺
TiO₂	0,08	± 0,005	—		—	
V	—		—		—	
Zn	0,165	± 0,004	0,0004	± 0,0001 ⁺	0,0051	± 0,0003 ⁺
Cl	—		0,095	± 0,006 ⁺	0,0173	± 0,0018 ⁺
Co	—		0,0019	± 0,0001 ⁺	(0,0016)	
Mo	—		0,0007	± 0,0001 ⁺	0,0020	± 0,0002 ⁺
Sn	—		0,0025	± 0,0002 ⁺	0,0006	± 0,0001 ⁺

(Values in parentheses are indicative values)

* 95%-confidence interval

Ceramic materials

Powder

Mass fraction in % $\pm$ standard

deviation

CRM-No.	D 777-1	D 779-1
Description	Silica brick	Magnesite, low boron
Year of issue	1984	1991
Si	44,44 $\pm$ 0,15	0,182 $\pm$ 0,015
SiO ₂	95,06 $\pm$ 0,32	–
Ca	2,02 $\pm$ 0,08	1,691 $\pm$ 0,023
CaO	2,83 $\pm$ 0,10	–
Mg	0,043 $\pm$ 0,007	(54,57)
MgO	0,071 $\pm$ 0,012	–
Al	0,42 $\pm$ 0,02	0,105 $\pm$ 0,007
Al ₂ O ₃	0,80 $\pm$ 0,04	–
B	–	0,0116 $\pm$ 0,0012
Cr	–	(0,0030)
Fe	0,23 $\pm$ 0,03	3,73 $\pm$ 0,06
Fe ₂ O ₃	0,33 $\pm$ 0,04	–
K	0,13 $\pm$ 0,02	(0,0020)
K ₂ O	0,15 $\pm$ 0,02	–
Mn	–	0,503 $\pm$ 0,017
Na	(0,02)	(0,0058)
P	–	0,0267 $\pm$ 0,0026
Ti	0,27 $\pm$ 0,02	0,0081 $\pm$ 0,0012

(Values in parentheses are indicative values)

Molybdenum oxide

Powder

CRM-No.	D 784-1
Description	Molybdenum oxide
Year of issue	2018
Ca	0,888 $\pm$ 0,008
Mg	0,0883 $\pm$ 0,0019
Ti	0,0223 $\pm$ 0,0010
P	0,0113 $\pm$ 0,0008
Bi	0,00326 $\pm$ 0,00020
Cu	0,390 $\pm$ 0,005
Fe	1,870 $\pm$ 0,021
Pb	0,0216 $\pm$ 0,0009
K	0,164 $\pm$ 0,007
Al	0,468 $\pm$ 0,010
As	0,0126 $\pm$ 0,0003
Mo	(57,87)
Si	(2,65)
S	(0,0088)
Na	(0,040)
C	(0,0103)
W	(0,015)
Ba	(0,006)
Co	(0,0045)
Ni	(0,0019)
Rb	(0,0006)
Sb	(0,0007)
Sr	(0,0041)
V	(0,127)
Zr	(0,0012)

Slags

Powder

Mass fraction in % $\pm$ standard deviation

CRM-No.	D 826-1	D 827-1
Description	Basic slag	Basic slag
Year of issue	1976	1976
SiO ₂	8,96 $\pm$ 0,15	6,21 $\pm$ 0,15
Al	0,696 $\pm$ 0,008	–
Al ₂ O ₃	–	(0,57)
CaO	46,48 $\pm$ 0,54	47,38 $\pm$ 0,49
MgO	(2,46)	(3,70)
P ₂ O ₅	14,65 $\pm$ 0,15	20,70 $\pm$ 0,16
P ₂ O ₅ citric acid sol.	10,73 $\pm$ 0,14	18,79 $\pm$ 0,22
B	(0,0029)	–
Cr	0,182 $\pm$ 0,005	–
Cr ₂ O ₃	–	(0,14)
Cu	(0,0019)	–
F	(0,3667)	–
Fe total	(20,73)	(15,72)
K	0,0278 $\pm$ 0,0017	–
Mn total	(3,46)	(2,34)
Mo	(0,0011)	–
Na	0,375 $\pm$ 0,009	–
Ni	(0,0017)	–
Pb	(0,0049)	–
V	0,503 $\pm$ 0,008	–
V ₂ O ₅	(0,89)	(1,15)

(Values in parentheses are indicative values)

Steels with certified oxygen and nitrogen content

Mass fraction in % $\pm$ standard deviation

CRM-No.	D 026-1	D 026-2	D 027-1	D 028-1
Description	Unalloyed steel	Unalloyed steel	Unalloyed steel	Unalloyed steel
Year of issue	1969	1973	1970	1970
Shape	Rods	Rods	Rods	Rods
O	0,0031 $\pm$ 0,0003	0,0025 $\pm$ 0,0004	0,0084 $\pm$ 0,0006	0,0113 $\pm$ 0,0007
N	0,0053 $\pm$ 0,0004	0,0042 $\pm$ 0,0003	0,0157 $\pm$ 0,0010	0,0029 $\pm$ 0,0005

CRM-No.	D 029-1	D 271-1	D 284-2	D 267-1
Description	Unalloyed steel	Stainless steel	Stainless steel	Stainless steel
Year of issue	1970	2007	2000	2021
Shape	Rods	Disc	Chips	Pins
O	0,0312 $\pm$ 0,0010	0,0020 $\pm$ 0,0002 ⁺	0,0099 $\pm$ 0,0007 ⁺	0,00096 $\pm$ 0,00009 ⁺
N	0,0083 $\pm$ 0,0008	0,0137 $\pm$ 0,0003 ⁺	0,0151 $\pm$ 0,0002 ⁺	0,0266 $\pm$ 0,0007 ⁺

(Values in parentheses are indicative values)

⁺ 95%-confidence interval

Setting-up sample for spectrometric analysis of low alloyed steels

BAM SUS-1 R

The setting-up sample is suitable for direct reading spark emission and X-ray fluorescence spectrometers analysing low alloyed steels.

The material was prepared by hot isostatic pressing (HIP) of powder which was atomised from the melt of the alloy and solidified in inert gas. Therefore it is of particular high homogeneity. Analysis of the sample was carried out in BAM.

Dimensions: cylinder, 50 mm in diameter, 42 mm high

Analyte	Uncertified mass fraction in %
C	0,9
Si	0,8
Mn	1,1
P	0,02
S	0,017
Cr	1,7
Mo	0,9
Ni	2,9
V	0,5
W	0,7
Cu	0,7
Co	0,3
Nb	0,55

Steel with certified hydrogen content

Mass fraction in mg/kg $\pm$ 95%-confidence interval

CRM-No.	CRM Steel-H2
Description	Alloyed steel, 1.4546.9
Year of issue	2022
Shape	Pins
H	1,26 $\pm$ 0,07

Non ferrous metals and alloys

The **aluminium, copper, lead and zinc based samples** were produced and certified by BAM in collaboration with the Working Groups „Aluminium“, „Copper“ and „Lead/Zinc“ of the Committee of Chemists of the Society of Metallurgists und Miners (GDMB).

The analyses were carried out in BAM and in laboratories of the non ferrous metals industry. The finely divided samples are supplied in glass bottles containing 100 g each.

Cylindrical samples in block form have been especially designed for spark emission and X-ray fluorescence spectrometers.

The **aluminium discs** are 2,5 to 5 cm high and 4 to 6 cm in diameter and have been analysed by 10 to 15 industrial laboratories (depending on the element) involved in an interlaboratory comparison organized by BAM.

The **copper blocks** of cylindrical shape have an approximate height of 3 cm and a diameter of about 4 cm.

Lead blocks of cylindrical shape have a height of 3 - 4 cm and a diameter of 4 - 5 cm.

Zinc blocks of cylindrical shape have a height of 3 cm and a diameter of about 4,5 cm.

The granulated **tin solder** was certified in a German-French collaboration by the Bureau National de Métrologie, involving several industrial laboratories of both countries. The sieved material (fraction 40 to 200 µm) is available from BAM in glass bottles containing 100 g each.

Each sample is distributed together with a certificate which contains the certified values together with their uncertainties and the indicative values. The mean values of the accepted data sets, their standard deviations and the standard deviations of the laboratories are also given in the certificate together with the laboratories participating in the certification campaign and the analytical methods used for element determination.

Authentic for the certified element contents are only the values given in the certificates, not the values given in this catalogue.

Aluminium

Chips, powder

Mass fraction in %

CRM-No.	201	300	301	BAM-M319 [□]
Description	GAISi12	AlMg3	Al99,8	AlMgSc
Year of issue	1963	1959	1961	2019
Al	(matrix)	(matrix)	(matrix)	(matrix)
Si	13,20	0,14	0,062	0,1043
Mg	0,0024	2,68	0,0008	4,96
Cu	0,009	0,040	0,0018	0,0015
Fe	0,18	0,198	0,054	0,291
Mn	0,38	0,018	(0,001)	0,371
Sc	–	–	–	0,847
Cr	–	0,216	–	(0,060)
Ga	–	–	–	(0,015)
Ni	–	–	–	(0,037)
Pb	–	–	–	(< 0,001)
Sn	–	(< 0,0005)	(< 0,0005)	(< 0,001)
Ti	0,011	0,012	0,0046	0,0030
V	–	–	0,0018	(0,0093)
Zn	0,038	0,128	0,036	0,0073
Zr	–	–	–	0,324

(Values in parentheses are indicative values)

□ Accredited by DAkkS as a producer of RM according to ISO 17034

Aluminium

Discs

Mass fraction in mg/kg (bold in %) ± estimated expanded uncertainty

CRM-No.	ERM®-EB307a	BAM-M308a ^Δ	BAM-310	ERM®-EB312a ^Δ	BAM-M313a ^Δ
Description	AlMg4,5Mn	AlZnMgCu1,5	Al99,85Mg1	AlMgSi0,5	AlMg3
Year of issue	2016	2018	1993	2017	2021
Si	0,152 ± 0,005	0,072 ± 0,003	0,0797 ± 0,0012 ⁺	0,403 ± 0,008	0,346 ± 0,012
Fe	0,345 ± 0,007	0,164 ± 0,005	0,0705 ± 0,0012 ⁺	0,198 ± 0,004	0,388 ± 0,010
Cu	0,0939 ± 0,0026	1,36 ± 0,03	16,9 ± 0,9 ⁺	0,0509 ± 0,0014	0,0932 ± 0,0027
Mn	0,811 ± 0,010	0,0343 ± 0,0005	30,7 ± 1,1 ⁺	0,0488 ± 0,0011	0,486 ± 0,006
Mg	4,80 ± 0,09	2,28 ± 0,05	0,994 ± 0,015 ⁺	0,379 ± 0,004	3,35 ± 0,08
Cr	0,1536 ± 0,0026	0,192 ± 0,004	0,90 ± 1,2 ⁺	0,0320 ± 0,0009	0,117 ± 0,004
Ni	0,0097 ± 0,0005	147 ± 3	24,4 ± 1,4 ⁺	40,7 ± 2,4	0,0296 ± 0,0007
Zn	0,0690 ± 0,0016	5,61 ± 0,08	86 ± 4 ⁺	0,0297 ± 0,0008	0,1481 ± 0,0026
Ti	0,0595 ± 0,0016	257 ± 7	30,1 ± 1,1 ⁺	0,0291 ± 0,0011	0,099 ± 0,006
Al	(matrix)	(matrix)	(matrix)	(matrix)	(matrix)
As	–	–	–	–	(3,8± 1,4)
B	–	–	(6)	(2,7± 1,0)	–
Be	5,37 ± 0,16	1,8 ± 0,1	1,28 ± 0,14 ⁺	–	5,4 ± 0,3
Bi	–	–	–	18,0 ± 1,8	92 ± 5
Ag	–	6,5 ± 0,6	–	–	–
Ca	19,2 ± 2,8	–	7,3 ± 0,4 ⁺	(16,9± 2,5)	10,4 ± 1,2
Cd	32,6 ± 1,4	–	23,7 ± 0,7 ⁺	16,7 ± 1,3	4,7 ± 0,6
Co	5,1 ± 0,5	–	(9)	–	–
Ga	0,0124 ± 0,0005	–	115,2 ± 2,4 ⁺	0,0129 ± 0,0003	106,7 ± 2,2
In	–	–	–	–	–
Hg	(34 ± 5)	–	–	–	3,7± 0,7
Li	8,1 ± 0,5	–	3,66 ± 0,12 ⁺	6,0 ± 1,1	11,3 ± 0,4
Mo	–	–	–	–	4,8± 0,8
Na	(8,4 ± 2,4)	15,8 ± 2,2	(3)	(4,0± 1,8)	25 ± 5
P	–	–	(3)	–	–
Pb	0,0084 ± 0,0004	43,6 ± 2,7	34,7 ± 2,5 ⁺	49,7 ± 2,1	38,0 ± 1,4
Sb	46 ± 6	–	–	–	6,1± 1,0
Sn	0,0075 ± 0,0004	–	23,8 ± 1,8 ⁺	–	193 ± 6
Sr	–	–	–	11,1± 0,7	–
Tl	–	–	–	–	(5,1± 0,6)
V	0,0119 ± 0,0004	–	44,4 ± 2,3 ⁺	67,3 ± 1,4	308 ± 8
Zr	31,9 ± 1,2	87,3 ± 2,6	13,5 ± 1,9 ⁺	8,5 ± 0,7	355 ± 10

(Values in parentheses are indicative values)

- continued -

⁺ 95% confidence interval

^Δ) Accredited by DAKS as a producer of RM in accordance with ISO Guide 34 in combination with ISO/IEC 17025

Aluminium, discs (continued)

Mass fraction in mg/kg (bold in %) ± estimated expanded uncertainty

CRM-No.	ERM®-EB314a	ERM®-EB315a ^Δ	BAM-M316a [□]	ERM®-EB317	BAM-M318 [□]
Description	AlSi11Cu2Fe	AlSi9Cu3	AlSi12(Fe)	AlZn6CuMgZr	AlSi1,2Mg0,4
Year of issue	2016	2017	2023	2013	2019
Si	11,51 ± 0,15	9,88 ± 0,18	11,87 ± 0,17	271 ± 22	1,211 ± 0,017
Fe	0,992 ± 0,017	0,621 ± 0,014	0,986 ± 0,018	0,112 ± 0,003	0,246 ± 0,008
Cu	2,08 ± 0,07	2,46 ± 0,08	0,0290 ± 0,0006	1,77 ± 0,06	0,0908 ± 0,0025
Mn	0,404 ± 0,008	0,311 ± 0,009	0,0240 ± 0,0008	912 ± 19	0,0985 ± 0,0017
Mg	0,196 ± 0,004	0,446 ± 0,023	0,0473 ± 0,0012	2,39 ± 0,07	0,356 ± 0,009
Cr	0,0574 ± 0,0012	0,0274 ± 0,0004	62,6 ± 1,4	0,141 ± 0,003	0,0208 ± 0,0004
Ni	0,242 ± 0,006	0,955 ± 0,0022	0,0251 ± 0,0007	359 ± 14	50,0 ± 1,9
Zn	1,100 ± 0,015	0,801 ± 0,010	0,0593 ± 0,0011	6,93 ± 0,26	0,0486 ± 0,0011
Ti	0,188 ± 0,004	0,142 ± 0,006	0,0791 ± 0,0014	952 ± 156	0,0238 ± 0,0010
Al	(matrix)	(matrix)	(matrix)	(matrix)	(matrix)
As	28 ± 7	–	–	–	–
B	–	(2,1 ± 2,0)	(2,5 ± 0,6)	(37 ± 32)	(< 2)
Be	4,65 ± 0,22	4,33 ± 0,16	4,6 ± 0,5	10,1 ± 0,8	4,7 ± 0,3
Bi	92 ± 6	36 ± 4	151 ± 6	41 ± 6	–
Ag	–	–	184 ± 6	73 ± 5	–
Ca	–	–	17,9 ± 1,4	(6,0 ± 2,7)	9,1 ± 1,6
Cd	5,2 ± 1,0	7,9 ± 1,0	19,5 ± 0,9	–	9,6 ± 1,2
Co	74 ± 4	(1,4 ± 0,7)	–	–	–
Ga	164 ± 4	0,0089 ± 0,0003	95,4 ± 2,0	183 ± 12	0,0189 ± 0,0005
In	–	–	–	162 ± 11	–
Hg	–	(22 ± 6)	(38 ± 5)	–	7,6 ± 1,1
Li	–	–	–	–	6,0 ± 0,7
Mo	–	–	–	–	–
Na	–	–	–	–	(3,7 ± 1,3)
P	–	(7 ± 4)	–	(27 ± 15)	–
Pb	0,189 ± 0,010	0,077 ± 0,003	89 ± 5	48,1 ± 2,3	56 ± 3
Sb	102 ± 19	51 ± 10	47 ± 4	–	–
Sn	0,201 ± 0,004	0,0764 ± 0,0020	100,5 ± 2,8	237 ± 18	20,6 ± 1,1
Sr	–	–	298 ± 8	–	–
Tl	–	–	–	–	–
V	277 ± 7	47,0 ± 2,3	98,4 ± 1,9	105 ± 7	0,0104 ± 0,0003
Zr	103 ± 3	31,0 ± 1,9	29,1 ± 1,5	0,130 ± 0,008	32,9 ± 1,4

(Values in parentheses are indicative values)

^Δ Accredited by DAkkS as a producer of RM in accordance with ISO Guide 34 in combination with ISO/IEC 17025

[□] Accredited by DAkkS as a producer of RM according to ISO 17034

Aluminium, discs (continued)

Mass fraction in mg/kg (bold in %) ± estimated expanded uncertainty

CRM-No.	BAM-M320 [□]	BAM-M321 [□]	BAM-M322 [□]	BAM-M323 [□]
Description	AlMgSc	AlCu4Mg1	AlMn1Cu	AlFe1
Year of issue	2020	2020	2021	2022
Si	0,197 ± 0,007	0,0496 ± 0,0020	0,696 ± 0,021	0,147 ± 0,005
Fe	0,206 ± 0,006	0,0495 ± 0,0017	0,475 ± 0,014	1,000 ± 0,012
Cu	0,147 ± 0,005	0,0908 ± 0,0025	0,200 ± 0,006	0,0182 ± 0,0004
Mn	0,699 ± 0,008	0,0985 ± 0,0017	1,310 ± 0,018	0,0471 ± 0,0009
Mg	3,98 ± 0,08	4,38 ± 0,06	0,226 ± 0,005	0,0203 ± 0,0013
Cr	0,1044 ± 0,0023	0,0558 ± 0,0013	0,1185 ± 0,0024	0,0106 ± 0,0003
Ni	20,9 ± 1,3	0,0504 ± 0,0007	0,0293 ± 0,0005	92,3 ± 2,7
Zn	0,252 ± 0,006	0,147 ± 0,003	0,1053 ± 0,0020	0,0286 ± 0,0006
Ti	0,102 ± 0,004	0,0436 ± 0,0022	0,0279 ± 0,0009	0,0188 ± 0,0006
Al	(matrix)	(matrix)	(matrix)	(matrix)
As	–	–	–	–
B	–	–	–	(2,6± 0,7)
Be	22,4 ± 0,7	4,9 ± 0,2	7,2 ± 0,2	5,3 ± 0,3
Bi	–	323 ± 14	76,5 ± 2,8	15,0 ± 1,7
Ag	–	–	–	–
Ca	11,9 ± 1,9	5,2 ± 0,8	19,9 ± 1,7	17 ± 4
Cd	15,2 ± 1,9	30 ± 4	10,1 ± 0,3	20,2 ± 0,9
Co	20,9 ± 1,2	–	9,7± 0,4	21,3± 1,3
Ga	0,0208 ± 0,0008	88,0 ± 2,0	57,7 ± 3,0	0,1410 ± 0,0006
In	–	–	–	–
Hg	–	–	–	19,9± 1,1
Li	9,1 ± 0,4	5,8 ± 0,4	18,1* ± 0,8	6,0* ± 0,7
Mo	–	–	–	–
Na	6,4 ± 1,3	2,9 ± 0,9	15,7* ± 1,1	8,8* ± 1,4
P	–	–	–	–
Pb	44,8 ± 2,4	99 ± 6	92,0 ± 2,5	44,1 ± 1,3
Sb	–	–	–	40± 4
Sc	0,282 ± 0,007	0,0502 ± 0,0020	–	–
Sn	45,6 ± 2,9	0,0286 ± 0,0010	97,7 ± 2,4	16,3 ± 0,6
Sr	–	–	–	–
Tl	–	–	–	–
V	75,9 ± 2,5	0,0105 ± 0,0003	114 ± 2,5	89,2 ± 2,9
Zr	0,102 ± 0,005	0,1554 ± 0,0026	98,0 ± 1,9	49,6 ± 1,4

(Values in parentheses are indicative values)

[□] Accredited by DAkkS as a producer of RM according to ISO 17034

* Mass fraction of Li and Na in BAM-M322 and BAM-M323 depending on sample number

Aluminium, discs (continued)

Mass fraction in mg/kg (bold in %) ± estimated expanded uncertainty

CRM-No.	BAM-M324 [□]	BAM-M325 [□]
Description	AlMg1Cu	AlSi7MgSr
Year of issue	2022	2023
Si	0,348 ± 0,005	6,83 ± 0,14
Fe	0,501 ± 0,007	0,143 ± 0,005
Cu	0,1983 ± 0,0026	0,0197 ± 0,0006
Mn	1,072 ± 0,011	0,0112 ± 0,0002
Mg	1,201 ± 0,019	0,504 ± 0,009
Cr	0,0258 ± 0,0005	63,4 ± 1,6
Ni	88,8 ± 2,1	47,8 ± 1,8
Zn	0,1761 ± 0,0022	0,0555 ± 0,0008
Ti	0,0371 ± 0,0007	0,117 ± 0,004
Al	(matrix)	(matrix)
As	–	–
B	9,8 ± 1,9	–
Be	8,7 ± 0,3	–
Bi	9,0 ± 1,3	–
Ag	–	–
Ca	13,7 ± 1,2	26 ± 4
Cd	45,4 ± 1,8	22,0 ± 1,0
Co	48,9 ± 1,3	–
Ga	0,0306 ± 0,0004	191 ± 5
In	–	–
Hg	7,2 ± 1,1	–
Li	10,1 ± 0,8	8,3 ± 1,5
Mo	–	–
Na	(9,0 ± 1,6)	(13,5 ± 2,8)
P	–	–
Pb	46,8 ± 2,0	104 ± 7
Sb	42 ± 6	37 ± 4
Sn	87,3 ± 1,8	183 ± 5
Sr	17,3 ± 1,4	301 ± 13
Tl	–	–
V	91,6 ± 2,8	95,7 ± 1,2
Zr	19,7 ± 1,0	56,9 ± 1,6

(Values in parentheses are indicative values)

[□] Accredited by DAkkS as a producer of RM according to ISO 17034

Copper

Chips

Mass fraction in % $\pm$ standard deviation

CRM-No.	223	224	227
Description	CuZn39Pb2	CuZn40MnPb	Rg7
Year of issue	1974	1975	1979
Cu	58,74 $\pm$ 0,02	57,40 $\pm$ 0,02	85,57 $\pm$ 0,03
Sn	0,089 $\pm$ 0,004	0,066 $\pm$ 0,003	6,01 $\pm$ 0,07
Zn	38,82 $\pm$ 0,09	39,40 $\pm$ 0,04	3,46 $\pm$ 0,03
Pb	2,13 $\pm$ 0,02	1,13 $\pm$ 0,04	4,12 $\pm$ 0,04
Fe	0,091 $\pm$ 0,002	0,136 $\pm$ 0,002	0,129 $\pm$ 0,002
Ni	0,0214 $\pm$ 0,0005	0,038 $\pm$ 0,001	0,284 $\pm$ 0,003
Mn	(< 0,001)	1,70 $\pm$ 0,03	–
Al	(< 0,002)	0,0012 $\pm$ 0,0002	(< 0,0001)
Ag	–	–	–
As	0,0084 $\pm$ 0,0005	0,0025 $\pm$ 0,0002	0,081 $\pm$ 0,002
Bi	0,0018 $\pm$ 0,0001	0,0006 $\pm$ 0,0001	0,0088 $\pm$ 0,0002
Cd	–	–	–
Co	–	–	–
P	0,0003 $\pm$ 0,00015	0,0112 $\pm$ 0,0002	(0,0002)
S	0,0011 $\pm$ 0,0001	0,0004 $\pm$ 0,0001	0,122 $\pm$ 0,005
Sb	0,0040 $\pm$ 0,0002	0,0026 $\pm$ 0,0001	0,160 $\pm$ 0,002
Se	(< 0,0001)	–	0,0028 $\pm$ 0,0002
Si	(< 0,003)	(0,002)	(< 0,01)
Te	–	–	0,0012 $\pm$ 0,0003

(Values in parentheses are indicative values)

- continued -

Copper, chips (continued)
Mass fraction in mg/kg (bold in %) ± uncertainty

CRM-No.	228	BAM-229	BAM-M365a ^Δ
Description	Rg10	CuZn37	Pure copper
Year of issue	1979	1996	2017
Cu	85,34 ± 0,03	63,334% ± 0,007 %	99,73 % ± 0,07 %
Zn	9,76 ± 0,05	36,63 % ± 0,04 %	30 ± 4
Sn	3,32 ± 0,05	48,5 ± 1,1	–
Pb	1,24 ± 0,03	192 ± 5	141 ± 4
Fe	0,036 ± 0,002	106,1 ± 2,1	6,1 ± 1,3
Ni	0,109 ± 0,005	111,4 ± 0,9	235 ± 5
Mn	(< 0,001)	–	–
Al	(0,0001)	–	–
Ag	–	–	159 ± 5
As	0,024 ± 0,001	21,7 ± 0,8	40,4 ± 0,8
Bi	0,0086 ± 0,0003	–	30,0 ± 1,2
Cd	–	–	–
Co	–	–	2,13 ± 0,14
P	0,019 ± 0,001	(10,6 ± 1,6)	–
S	0,036 ± 0,002	–	–
Sb	0,078 ± 0,001	7,2 ± 0,7	12,1 ± 1,0
Se	0,0012 ± 0,0001	34 ± 4	179 ± 12
Si	–	–	–
Te	–	–	1,27 ± 0,12

(Values in parentheses are indicative values)

^Δ) Accredited by DAkkS as a producer of RM in accordance with ISO Guide 34 in combination with ISO/IEC 17025

Copper

Discs

Mass fraction in mg/kg (bold in %) ± uncertainty

CRM-No.	BAM-368	BAM-369	BAM-370	BAM-371	BAM-372	ERM®-EB374 (BAM-374)
Description	CuZn20Al2	OF-Cu	OF-Cu	OF-Cu	OF-Cu	CuSn8
Year of issue	1993	1993	1993	1995	1995	1999
Cu	77,049 ± 0,018	(matrix)	(matrix)	(matrix)	(matrix)	92,22 ± 0,05
Al	1,972 ± 0,014	—	12,6 ± 0,8	—	—	(< 1)
Ni	258 ± 4	—	—	—	11,66 ± 0,24	32,7 ± 1,3
Fe	192,7 ± 2,9	—	—	18,3 ± 0,7	—	40 ± 4
Mn	202,8 ± 2,4	—	—	—	11,4 ± 0,4	4,3 ± 0,3
Zn	(matrix)	22,0 ± 0,6	—	—	—	40,4 ± 1,9
Ag	—	—	—	—	9,01 ± 0,29	12,1 ± 1,3
As	246 ± 9	—	—	—	10,3 ± 0,6	(4,3 ± 1,2)
Be	—	—	—	11,5 ± 0,6	—	—
Bi	—	9,7 ± 0,4	—	—	—	(2,2 ± 1,3)
C	—	—	—	—	—	—
Cd	—	—	—	1,63 ± 0,08	—	(< 1)
Co	—	10,42 ± 0,29	—	—	—	(< 1)
Cr	—	9,2 ± 0,5	—	—	—	(< 1)
Mg	62,1 ± 1,5	3,60 ± 0,18	—	—	—	(< 1)
P	89,9 ± 1,6	—	11,7 ± 0,7	—	—	0,170 ± 0,008
Pb	131,3 ± 2,4	—	15,8 ± 1,1	—	—	8,3 ± 0,9
S	(18,5 ± 2,9)	—	—	12,1 ± 0,9	—	(13 ± 5)
Sb	—	—	15,6 ± 1,3	—	—	(6,3 ± 1,4)
Se	—	—	—	—	(8,4 ± 0,6)	(< 2)
Si	130 ± 7	—	18,7 ± 3,0	—	—	(< 10)
Sn	147 ± 4	—	16,8 ± 0,9	—	—	7,60 ± 0,13
Te	—	—	—	14,4 ± 0,6	—	(< 1)
Ti	—	—	—	12,9 ± 0,7	—	(< 1)
Zr	—	—	—	—	5,8 ± 0,4	(< 1)

(Values in parentheses are indicative values)

- continued -

Copper, discs (continued)

Mass fraction in mg/kg (bold in %) ± estimated expanded uncertainty

CRM-No.	BAM-M376a	ERM®-EB377 (BAM-377)	ERM®-EB378 (BAM-378)	BAM-M381
Description	Pure copper	CuSn6	CuSn6	Pure copper
Year of issue	2016	1999	2000	2006
Cu	(matrix)	94,04 ± 0,05	94,13 ± 0,04	(matrix)
Al	(182 ± 10)	45,1 ± 1,2	(< 1)	(< 1)
Ni	209 ± 6	107,4 ± 1,5	18,3 ± 0,9	0,7 ± 0,2
Fe	235 ± 3	104,2 ± 2,7	182 ± 7	3,3 ± 0,2
Mn	206 ± 3	92,1 ± 2,1	(0,74 ± 0,24)	0,22 ± 0,03
Zn	217 ± 3	100,6 ± 3,0	(7,4 ± 1,0)	5,3 ± 0,3
Ag	163 ± 3	64,4 ± 1,1	26,6 ± 1,3	< 1
As	200 ± 3	(< 10)	99,5 ± 2,5	< 0,5
Be	(41 ± 6)	–	–	–
Bi	200 ± 5	42,2 ± 1,5	(< 1)	< 0,3
C	–	–	–	–
Cd	186,1 ± 3	(< 1)	100,7 ± 2,2	< 0,4
Co	208 ± 2	(< 2)	89 ± 5	< 0,3
Cr	(400 ± 60)	66,9 ± 2,1	311 ± 5	< 0,4
Ge	–	–	–	–
In	–	–	–	–
Mg	(124 ± 19)	(< 1)	28,7 ± 0,8	< 0,6
P	203 ± 5	(< 10)	602 ± 23	–
Pb	236 ± 4	44,9 ± 2,3	4,2 ± 0,7	0,59 ± 0,07
S	(133 ± 19)	(6,8 ± 0,8)	9,1 ± 1,9	(3,2 ± 1,3)
Sb	202 ± 5	13,0 ± 1,3	86,1 ± 2,6	< 1
Se	210 ± 4	55 ± 4	(< 2)	(< 1)
Si	–	(134)	(< 10)	(< 3)
Sn	247 ± 3	5,92 ± 0,13	5,74 ± 0,21	3,86 ± 0,25
Te	215 ± 7	(< 1)	85,0 ± 2,6	(< 0,3)
Ti	(4,5 ± 1,7)	(< 1)	(29,4 ± 4)	(< 0,3)
Zr	42,2 ± 1,9	–	(1,7 ± 0,09)	< 6

(Values in parentheses are indicative values)

- continued -

Copper, discs (continued)

Mass fraction in mg/kg ± estimated expanded uncertainty

CRM-No.	BAM-M382a ^Δ	BAM-M383d [□]	BAM-M384b	BAM-M384c [□]
Description	Pure copper	Pure copper	Pure copper	Pure copper
Year of issue	2021	2021	2014	2022
Cu	(matrix)	(matrix)	(matrix)	(matrix)
Al	< 2	< 1,0	(2,9 ± 0,8)	< 2
Ni	2,7 ± 0,3	4,7 ± 0,4	4,7 ± 0,6	5,7 ± 0,5
Fe	10,3 ± 0,7	22,4 ± 0,9	(5,1 ± 1,2)	33,0 ± 1,1
Mn	2,5 ± 0,2	0,97 ± 0,09	8,1 ± 0,9	5,7 ± 0,5
Zn	7,6 ± 0,6	1,08 ± 0,14	2,6 ± 0,5	1,0 ± 0,3
Ag	2,9 ± 0,2	10,2 ± 0,3	11,3 ± 0,4	14,8 ± 0,5
As	0,73 ± 0,12	1,20 ± 0,11	6,6 ± 1,1	2,9 ± 0,3
Be	–	–	–	–
Bi	0,75 ± 0,11	0,82 ± 0,07	6,81 ± 0,23	3,8 ± 0,3
C	–	–	–	–
Cd	0,50 ± 0,05	0,62 ± 0,05	4,0 ± 0,2	5,0 ± 0,4
Co	0,92 ± 0,08	1,30 ± 0,06	10,4 ± 0,5	4,0 ± 0,2
Cr	0,24 ± 0,07	0,77 ± 0,12	(2,3 ± 0,6)	(4,7 ± 0,8)
Mg	1,9 ± 0,3	1,7 ± 0,2	3,3 ± 0,5	1,8 ± 0,4
P	(< 2)	< 1,0	(< 2)	< 1
Pb	2,2 ± 0,5	7,8 ± 1,0	1,6 ± 0,4	7,2 ± 0,6
S	6,7 ± 1,0	3,5 ± 0,6	(3,8 ± 1,4)	4,0 ± 0,4
Sb	0,87 ± 0,14	1,8 ± 0,2	5,8 ± 0,4	9,8 ± 0,6
Se	0,77 ± 0,07	(0,6 ± 0,4)	(2,9 ± 0,7)	2,9 ± 0,4
Si	–	–	(<2,5)	–
Sn	4,7 ± 0,4	3,8 ± 0,4	2,1 ± 0,4	0,6 ± 0,1
Te	0,72 ± 0,08	0,47 ± 0,05	7,2 ± 0,7	6,1 ± 0,7
Ti	0,57 ± 0,06	1,2 ± 0,3	2,9 ± 0,6	< 0,2
Zr	(< 1)	< 1,0	1,3 ± 0,4	< 0,3

(Values in parentheses are indicative values)

^Δ Accredited by DAkkS as a producer of RM in accordance with ISO Guide 34 in combination with ISO/IEC 17025

[□] Accredited by DAkkS as a producer of RM according to ISO 17034

- continued -

Copper, discs (continued)

Mass fraction in mg/kg (bold in %) ± estimated expanded uncertainty

CRM-No.	BAM-M386a [□]	ERM [®] -EB387 (BAM-M387)	ERM [®] -EB388 (BAM-M388)	ERM [®] -EB389	ERM [®] -EB393a
Description	Pure copper	CuZn20Ni5	CuAl5Zn5Sn	CuNi25	CuZn21Si3P
Year of issue	2021	2004	2004	2007	2016
Cu	(matrix)	75,18 ± 0,04	89,27 ± 0,05	74,3 ± 0,5	75,8 ± 0,3
Al	26,9 ± 2,3	–	4,972 ± 0,024	(123 ± 10)	2,1 ± 0,4
Ni	21,1 ± 1,1	5,020 ± 0,025	73,6 ± 2,0	24,7 ± 0,5	29,7 ± 1,5
Fe	59,3 ± 1,3	617 ± 10	303 ± 9	0,107 ± 0,006	143 ± 5
Mn	11,1 ± 0,6	796 ± 6	512 ± 6	0,415 ± 0,011	18,5 ± 0,6
Zn	36,7 ± 1,5	19,57 ± 0,06	4,81 ± 0,03	0,1125 ± 0,0026	(20,8)
Ag	44,2 ± 1,4	–	–	–	–
As	20,8 ± 0,8	–	–	–	1,34 ± 0,16
B	–	–	–	(23 ± 6)	–
Be	–	–	–	–	–
Bi	9,5 ± 0,5	–	–	44 ± 10	(0,19 ± 0,05)
C	–	–	–	(216 ± 24)	–
Cd	5,4 ± 0,5	–	–	16 ± 3	0,61 ± 0,17
Co	4,9 ± 0,3	–	–	770 ± 28	–
Cr	11,5 ± 0,9	–	–	153 ± 6	1,56 ± 0,28
Mg	76,7 ± 2,8	–	–	0,067 ± 0,009	–
P	6,5 ± 0,7	–	–	93 ± 17	0,0454 ± 0,0012
Pb	19,8 ± 1,1	10,8 ± 0,8	9,69 ± 0,83	98 ± 23	104 ± 4
S	15,9 ± 1,8	–	–	(308 ± 23)	–
Sb	25,2 ± 1,8	–	–	46 ± 5	(0,93 ± 0,29)
Se	9,7 ± 0,9	–	–	–	(0,47 ± 0,15)
Si	–	–	–	(349 ± 37)	3,35 ± 0,06
Sn	21,6 ± 0,9	30,1 ± 1,2	0,857 ± 0,011	262 ± 34	39,0 ± 0,9
Te	31,1 ± 1,3	–	–	–	–
Ti	34,7 ± 1,4	–	–	660 ± 18	–
Zr	–	–	–	0,098 ± 0,011	–

(Values in parentheses are indicative values)

CRM-No.	BAM-M390	BAM-M391	BAM-M392
Description	Pure copper	Pure copper	Pure copper
Year of issue	2010	2010	2010
Fe	0,79 ± 0,20	0,90 ± 0,21	0,80 ± 0,17
P	1,3 ± 0,4	3,3 ± 0,5	7,0 ± 0,5
Sn	(< 0,1)	(< 0,1)	(< 0,1)

(Values in parentheses are indicative values)

Copper, discs (continued)

Mass fraction in mg/kg (bold in %) ± estimated expanded uncertainty interval

CRM-No.	BAM-M394 ^A	BAM-M394a ^A	BAM-M396 [□]	BAM-M397 [□]	BAM-M397a [□]
Description	CuZn40Pb2	CuZn40Pb2	CuZn33Pb1AlSiAs	CuSn4Zn2PS	CuSn4Zn2PS
Year of issue	2017	2017	2019	2019	2019
Cu	57,70 ± 0,19	57,64 ± 0,17	65,49 ± 0,12	–	–
Al	(1,0 ± 1,1)	(7,9 ± 1,4)	0,223 ± 0,010	–	–
Ni	399 ± 8	386 ± 7	143 ± 17	0,336 ± 0,006	0,337 ± 0,007
Fe	0,1191 ± 0,0024	0,1323 ± 0,0026	0,0235 ± 0,0012	–	–
Mn	14,1 ± 0,7	12,5 ± 0,7	44,5 ± 1,9	–	–
Zn	–	–	–	1,96 ± 0,05	1,87 ± 0,06
Ag	–	–	–	–	–
As	100,1 ± 2,6	95,9 ± 1,6	0,0590 ± 0,0016	(2,9 ± 0,3)	(2,9 ± 0,2)
B	–	–	–	–	–
Be	–	–	–	–	–
Bi	8,1 ± 0,9	8,3 ± 1,0	3,2 ± 0,03	–	–
C	–	–	–	–	–
Cd	7,0 ± 0,4	7,3 ± 0,6	2,2 ± 0,2	–	–
Co	–	–	1,2 ± 0,1	–	–
Cr	(< 2)	1,3 ± 0,3	7,9 ± 0,7	–	–
Mg	–	–	–	–	–
P	15,7 ± 1,2	17,2 ± 1,6	8,9 ± 1,0	–	–
Pb	1,93 ± 0,04	1,92 ± 0,04	0,592 ± 0,014	0,229 ± 0,008	0,227 ± 0,008
S	–	–	–	0,459 ± 0,029	0,45 ± 0,04
Sb	23,8 ± 1,3	24,1 ± 1,0	6,1 ± 0,7	0,097 ± 0,004	0,097 ± 0,004
Se	–	–	(< 10)	(<1)	(<1)
Si	(5,5 ± 5,2)	(5,8 ± 4,1)	0,187 ± 0,008	–	(<1)
Sn	0,232 ± 0,006	0,174 ± 0,006	0,0367 ± 0,0011	3,99 ± 0,08	3,98 ± 0,10
Te	–	–	–	–	–
Ti	–	–	–	(<1)	–
Zr	–	–	–	–	–

(Values in parentheses are indicative values)

□ Accredited by DAkkS as a producer of RM according to ISO 17034

^A) Accredited by DAkkS as a producer of RM in accordance with ISO Guide 34 in combination with ISO/IEC 17025

Tin-lead solder

Granulated powder

Mass fraction in % $\pm$ 95%-confidence interval

CRM-No.	BNM 010	
Description	Sn63Pb37	
Year of issue	1991	
Sn	63,40	$\pm 0,07$
Pb	36,47	$\pm 0,17$
Bi	0,0245	$\pm 0,0010$
Cd	0,0016	$\pm 0,0002$
Cu	0,0417	$\pm 0,0014$
Ni	0,0021	$\pm 0,0002$
Sb	0,0488	$\pm 0,0008$
Ag	(0,014)	
As	(0,012)	
Au	(< 0,001)	
Fe	(0,0020)	
In	(< 0,001)	
Zn	(< 0,0001)	

(Values in parentheses are indicative values)

Precious metal alloys

Slices

Mass fraction in % ± estimated expanded uncertainty ($k=2,5$)

CRM-No.	ERM®-EB506	ERM®-EB507	ERM®-EB508
Description	rose gold	white gold	yellow gold
Year of issue	2014	2014	2014
Au	58,56 ± 0,06	75,10 ± 0,11	75,12 ± 0,11
Ag	3,90 ± 0,05	3,02 ± 0,05	24,90 ± 0,05
Cu	35,65 ± 0,06	14,69 ± 0,05	—
Ni	—	4,99 ± 0,04	—
Zn	1,891 ± 0,018	2,107 ± 0,016	—

Zinc

Disc

Mass fraction in mg/kg ± 95%-confidence interval

CRM-No.	BAM-M601
Description	Pure zinc
Year of issue	2005
Cd	0,55 ± 0,06
Fe	2,20 ± 0,09
Cu	1,89 ± 0,11
Tl	2,25 ± 0,09
Pb	15,7 ± 0,3
Al	< 0,5
In	< 0,05

Zinc-alloy

Disc

Mass fraction in mg/kg (bold in %)
± estimated expanded uncertainty ($k=2$) (Fe: $k=3$)

CRM-No.	ERM®-EB602
Description	ZnAl4Cu1
Year of issue	2014
Al	4,08 ± 0,11
Cu	0,812 ± 0,017
Mg	0,0415 ± 0,0020
Pb	19,5 ± 3,0
Cd	1,1 ± 0,5
Fe	7,3 ± 1,6
Sn	1,0 ± 0,5
Ni	2,5 ± 0,4
Si	11,4 ± 1,9
Ti	4,8 ± 0,4

Zinc powder

BAM-M603[□]

Year of issue: 2019

Certified values			Informative values		
Element	Mass fraction in mg/kg	Uncertainty in mg/kg	Element	Mass fraction in mg/kg	Uncertainty in mg/kg
Pb	15,8	0,5	Al	0,22	0,15
Ag	1,00	0,09	Bi	0,102	0,002
Cd	1,69	0,12	Co	0,041	0,004
Cu	3,69	0,21	Sb	0,04	0,02
Fe	2,18	0,14	As	<1	—
Ni	0,43	0,05	In	<0,5	—
Tl	3,81	0,23	Sn	<1	—
			V	<0,2	—

[□] Accredited by DAkkS as a producer of RM according to ISO 17034

Zinc/Aluminum alloys, discs

for the determination of chemical composition and sputter factor (GDOES); Year of issue: 2020

Mass fraction in % (bold in mg/kg) ± estimated expanded uncertainty ($k = 2$)

CRM-No.	AlZn-G1	AlZn-G2	AlZn-G3	AlZn-G4	AlZn-G5	AlZn-G6
Description	Zn99.95	Zn99.9	Zn99.7	Zn99.7	Zn99	Zn97
Al	494 ± 24	0,101 ± 0,004	0,151 ± 0,004	0,198 ± 0,004	0,264 ± 0,011	0,894 ± 0,023
Fe	71 ± 4	0,0222 ± 0,0006	0,0416 ± 0,0003	0,0732 ± 0,0006	0,0907 ± 0,0023	0,146 ± 0,004
Si	–	–	–	–	–	–
Pb	21,2 ± 1,2	0,00218 ± 0,00017	0,00214 ± 0,00012	0,00197 ± 0,00014	0,053 ± 0,004	–
Mg	–	–	–	–	0,43 ± 0,03	1,83 ± 0,18
Zn	–	–	–	–	–	–
Sputter factor	(7,21)	(6,25)	(6,08)	(5,77)	(4,97)	(4,48)
Density/g cm ⁻³	(7,13)	(7,12)	(7,12)	(7,11)	(7,01)	(6,70)

CRM-No.	AlZn-G7	AlZn-G8	AlZn-G9	AlZn-G10	AlZn-11
Description	Zn93Al4Mg3	Zn95Al5	Zn80Al20	Zn48Al50	Zn44Al55
Al	3,91 ± 0,07	4,85 ± 0,16	19,5 ± 0,4	49,5 ± 1,3	55,2 ± 1,1
Fe	0,0057 ± 0,0003	0,0074 ± 0,0007	0,082 ± 0,005	0,594 ± 0,011	0,502 ± 0,011
Si	–	–	(0,246)	(1,463)	0,99 ± 0,09
Pb	–	0,100 ± 0,005	0,00214 ± 0,00012	–	–
Mg	3,28 ± 0,11	–	–	–	–
Zn	–	–	–	(48,4)	(43,3)
Sputter factor	(3,80)	(3,52)	(1,97)	(0,81)	(0,72)
Density/g cm ⁻³	(6,19)	(6,59)	(5,36)	(3,87)	(3,70)

(Values in parentheses are indicative values)

Lead-alloys, discs

Mass fraction in mg/kg (bold in %) ± estimated expanded uncertainty ($k=2$)

CRM-No.	ERM®-EB102a
Description/ year of issue	PbCaSn/ 2009
Ca	0,0635% ± 0,0022%
Sn	1,01 % ± 0,05 %
Al	124 ± 11
Ag	170 ± 6
Bi	73,7 ± 2,6
Cu	1,3 ± 0,4
Sb	(4 ± 4)
As	(< 2)
Se	–
Tl	30,2 ± 1,5
Ni	–
P	–
Cd	–
S	(< 3)
In	(< 2)
Te	(< 1,1)
Zn	(< 0,5)
Fe	(< 2)
Mg	(< 1)
Na	(4 ± 1)

(Values in parentheses are indicative values)

Lead, lead alloys, discs

Mass fraction in mg/kg (bold in %) ± estimated expanded uncertainty (k=2)

CRM-No.	ERM®-EB104	ERM®-EB105	ERM®-EB106
Description	PbCaSn	PbCaSn	PbCaSn
Year of issue	2011	2011	2011
Ca	0,0530% ± 0,0018%	0,0595% ± 0,0016%	0,0782% ± 0,0026%
Sn	1,27 % ± 0,007 %	1,43 % ± 0,07 %	1,72 % ± 0,05 %
Ag	(29,3)	32,1 ± 0,9	(32,3)
Bi	(126)	133 ± 5	(135)

(Values in parentheses are indicative values)

Mass fraction in mg/kg ± estimated expanded uncertainty (k=2)

CRM-No.	ERM®-EB107	ERM®-EB108
Description	Pure lead	Pure lead
Year of issue	2015	2015
Cd	26,1 ± 1,1	26,0 ± 1,3
Hg	11,3 ± 0,9	8,3 ± 0,9

Mass fraction in mg/kg (bold in %) ± estimated expanded uncertainty (k=2)

CRM-No.	BAM-M109 ^A	BAM-M110 ^A	BAM-M112 ^A
Description	Refined lead	PbSb3	Pure lead
Year of issue	2018	2018	2020
As	0,0113 ± 0,0006	0,107 ± 0,008	–
Bi	0,0193 ± 0,0006	0,0126 ± 0,0004	(70)
Sb	0,0098 ± 0,0003	3,08 ± 0,08	–
Se	–	0,0106 ± 0,0014	–
Sn	0,115 ± 0,004	0,131 ± 0,004	5,2 ± 0,4
Ag	45,1 ± 1,0	22,6 ± 1,7	(8)
Cd	35,3 ± 0,9	–	–
Cu	19,6 ± 0,7	6,4 ± 0,4	8,2 ± 0,6
Ni	3,5 ± 0,3	–	5,3 ± 0,4
Te	30,6 ± 1,5	3,8 ± 0,9	5,3 ± 0,3
Tl	3,0 ± 0,5	–	(13)
Zn	31,8 ± 2,1	(<1)	–
Al	(<2,1)	–	–
In	(<0,5)	–	–
Pt	–	–	5,4 ± 0,5

(Values in parentheses are indicative values)

^{A)} Accredited by DAkkS as a producer of RM in accordance with ISO Guide 34 in combination with ISO/IEC 17025

Special materials

Glass

The CRMs in the field of **high tech ceramics** and of **refractory metals** were produced and certified by BAM in collaboration with the Working Group "Special Materials" of the Committee of Chemists of the Gesellschaft für Bergbau, Metallurgie, Rohstoff- und Umwelttechnik (GDMB). The analyses were carried out in BAM and in national and international laboratories of producers and users of these materials and of research institutes. The powder samples are supplied in tightly closed glass bottles containing 50 g or 100 g each.

The **glass** CRMs were produced and certified by BAM in collaboration with the Technical Committee 2 of the International Commission on Glass (ICG, TC-2). The analyses were carried out in BAM and in the laboratories of international members of ICG, TC-2 and some other laboratories. All laboratories are from glass making industry or from glass research institutes. The crushed glass sample (BAM-S004) is supplied in glass bottles containing 50 g each.

The **pure substances** are intended for analyte calibration and matrix simulation of atomic spectrometric methods, especially for X-ray fluorescence analysis (XRF). The samples were prepared and certified by Arbeitsgemeinschaft "Zertifiziertes Referenzmaterial Eisen und Stahl" (BAM, VDEh, MPI für Eisenforschung), Working Group "Primary substances for calibration". They can be ordered in polyethylene bottles with a unit size of 100 g. Each sample is distributed together with a certificate which contains the certified values together with their uncertainties (95%-level, if necessary extended by contributions from sample inhomogeneity) and the indicative values. The mean values of the accepted data sets, their standard deviations and the standard deviations of the mean values of laboratories are also given in the certificate together with the laboratories participating in the certification campaign and the analytical methods used for determination of element mass fractions or other parameters.

The material **BAM-H010** intended for use in quality assurance of measurements of elements in polymers and related matrices in order to support e.g. the EU directive 2002/95/EG (RoHS). The development and production of the acrylonitrile-butadiene-styrene terpolymer (ABS) has been carried by the Fachhochschule Münster. The certification process has been carried out by BAM. The reference material is available in form of granulate (100 g) or as discs with a diameter of 4 cm and a thickness of 1, 2 or 6 mm.

High tech ceramics Boron carbide powder

ERM®-ED102

Analyte	Certified value	Uncertainty *	Unit of mass fraction
Al	157	5	mg/kg
Ca	97	8	mg/kg
Co	0,39	0,09	mg/kg
Cr	5,6	1,2	mg/kg
Cu	2,2	0,4	mg/kg
Fe	686	22	mg/kg
Mn	10,4	0,5	mg/kg
Na	6,3	0,9	mg/kg
Ni	8,0	1,6	mg/kg
Si	268	22	mg/kg
Ti	96	5	mg/kg
Zr	48,9	2,3	mg/kg
C total	21,01	0,28	%
O	0,10	0,04	%
N	0,209	0,026	%
B total	78,47	0,31	%
B soluble	0,116	0,013	%
B ₂ O ₃	0,075	0,023	%
¹⁰ B ¹⁾	19,907	0,014	Isotopic abundance in %
	Indicative value	Uncertainty *	Unit of mass fraction
Mg	3,2	1,0	mg/kg
W	3,6	2,1	mg/kg
C free	0,51	0,12	%

* The uncertainty is the expanded uncertainty estimated in accordance with the Guide to the Expression of Uncertainty in Measurements (GUM) with a coverage factor of $k=2$.

¹⁾ Isotopic abundance (amount fraction) of ¹⁰Boron related to total amount of Boron.

Boron nitride powder

ERM®-ED103		
Analyte	Certified value in mg/kg	Uncertainty ¹⁾ in mg/kg
Al	7,0	1,4
Ca	273	16
Cr	4,7	1,1
Fe	15,0	2,2
Mg	56	5
Na	12,3	1,0
Si	17	4
Ti	4,9	0,7
Co	(<0,1)	—
	in %	in %
O	0,68	0,19
N	55,6	0,6
B total	43,5	0,5
B ₂ O ₃ adherent	0,070	0,014
C	(0,018)	(0,009)
H ₂ O	(<0,1)	—

Silicon nitride powder

ERM®-ED101		
Analyte	Certified value in mg/kg	Uncertainty ¹⁾ in mg/kg
Al	469	12
Ca	14,1	0,5
Co	43,5	0,8
Fe	79,5	1,3
Mg	4,3	0,4
Na	7,59	0,27
W	41,3	1,3
	in %	in %
C	0,162	0,024
N	38,1	0,2
O	(1,91)	(0,07)
β-phase	7,43	0,09

(Values in parentheses are indicative values)

¹⁾ The certified uncertainty is the expanded uncertainty estimated in accordance with the Guide to the Expression of Uncertainty in Measurements (GUM) with a coverage factor $k = 2$. It includes contributions from sample inhomogeneity and sample stability.

Yttrium stabilized zirconium oxide

ERM®-ED105

Analyte	Certified value ¹⁾	Uncertainty ²⁾	Unit of mass fraction
Al	660	15	mg/kg
Ca	242	9	mg/kg
Fe	95	9	mg/kg
Mg	12,9	1,7	mg/kg
Si	195	40	mg/kg
Th	112	17	mg/kg
Ti	497	11	mg/kg
U	292	19	mg/kg
Hf	1,535	0,024	%
Y	6,11	0,09	%
O	25,2	0,4	%
P	(< 75)	–	mg/kg
N	(912)	(140)	mg/kg
ZrO ₂ (monoclinic)	(1,94)	–	%

(Values in parentheses are indicative values)

¹⁾ The certified values are the means of 11-20 series of results (depending on the parameter) obtained by different laboratories. Up to 7 different analytical methods were used for the measurement of each parameter. The methods applied for determination of element mass fractions were calibrated using pure substances of definite stoichiometry or solutions prepared from them, thus achieving traceability to the International System of Units (SI).

²⁾ The uncertainty of the certified value is the expanded uncertainty estimated in accordance with the Guide to the Expression of Uncertainty in Measurement (GUM) with a coverage factor $k = 2$. It includes contributions from sample inhomogeneity.

Silicon carbide powder

Analyte	BAM-S003a (green micro F 800)		BAM-S008 (transparent 200/F)	
	Mass fraction mg/kg	Uncertainty mg/kg	Mass fraction mg/kg	Uncertainty mg/kg
Al	372	20	47	7
B	63	7	3,0	1,2
Ca	29,4	2,7	0,25	0,6
Cr	3,5	0,4	0,16	0,05
Cu	1,5	0,4	0,10	0,05
Fe	149	15	4,8	0,8
Mg	6,3	0,9	0,07	0,07
Mn	1,44	0,25	0,05	0,02
Na	17,7	0,8	0,17	0,09
Ni	32,9	2,7	0,9	0,5
Ti	79	4	67	6
V	41	5	275	18
Zr	25,2	2,0	4,4	1,2
C _{free}	493	79	–	–
O	(910)	(53)	146	36
N	(93)	(22)	18	4
SiO ₂ free	(600)	(148)	–	–
Si _{free}	(481)	(223)	–	–
	Mass fraction %	Uncertainty %	Mass fraction %	Uncertainty %
C _{total}	29,89	0,07	29,9	0,1
C _{free}	–	–	0,045	0,010

(Values in parentheses are indicative values)

Tungsten metal powder

BAM-S002

Analyte	Mass fraction mg/kg	Uncertainty mg/kg
Al	29,4	0,9
Ca	46	4
Co	45	6
Cr	47,0	1,4
Cu	28,4	2,9
Fe	53	5
K	40,0	1,8
Mg	38,8	2,7
Mn	16,7	1,9
Mo	59	4
Na	41	5
Ni	29	4
P	(7,2)	(1,3)
Si	106	10
Sn	42	6

(Values in parentheses are indicative values)

Titanium diboride powder

BAM-S012

Parameter	Certified values		Parameter	Informative values	
	Mass fraction in %	Uncertainty in %		Mass fraction in %	Uncertainty in %
Ti	68,3	0,8	C	0,169	0,008
B	30,71	0,15	N	0,120	0,007
B ₂ O ₃	0,359	0,024	O	0,48	0,08
			R _{acid}	0,22	0,03
	in mg/kg			in mg/kg	
Al	12,0	1,3	Si	11	5
Ca	44	4	Na	< 10	–
Cr	97	4	Nb	1700	–
Fe	640	40	S	2	–
Mg	1,6	0,4	W	114	–
Mn	3,8	0,4	Particle size distribution determined by laser light diffraction method		
Mo	11,7	0,7			
Ni	23,5	1,1			
V	10,2	0,8	D ₉₇	33,8 µm	
Zr	121	4	D ₅₀	12,3 µm	
			D ₀₆	2,3 µm	

Niobium pentoxide

BAM-S011

Parameter	Mass fraction mg/kg	Uncertainty mg/kg
F	128	13
Al	(0,29)	(0,16)
Cr	(0,031)	(0,005)
Cu	(0,040)	(0,009)
Fe	(0,26)	(0,08)
Ta	(8)	(6)
Mo	(< 0,05)	–
Ni	(< 0,3)	–
Particle size	Value in μm	
d ₁₀	(0,87)	–
d ₅₀	(2,2)	–
d ₉₀	(18,1)	–

(Values in parentheses are informative values)

Niobium carbide powder

BAM-S013

Parameter	Certified values		Parameter	Informative values	
	Mass fraction in %	Uncertainty in %		Mass fraction in %	Uncertainty in %
C	10,66	0,07	C _{free}	0,10	0,04
O	0,307	0,013	N	0,0031	0,0009
			S	0,0017	0,0005
			H	0,0076	0,0007
			Particle size distribution determined by laser light diffraction method		
			D ₁₀	1,10 μm	0,23 μm
			D ₅₀	3,57 μm	0,18 μm
			D ₉₀	6,7 μm	0,4 μm

Li-NMC 111 Cathode Material

BAM-S014

Parameter	Certified values		Parameter	Informative values	
	Mass fraction in %	Uncertainty in %		Mass fraction in %	Uncertainty in %
Li	7,62	0,16	C _{free}	0,10	0,04
Ni	19,76	0,13	N	0,0031	0,0009
Mn	18,22	0,14	S	0,0017	0,0005
Co	19,80	0,12			
O	34,0	1,0			
	in mg/kg			in mg/kg	
Al	14,1	1,9	P	12,2	2,2
C	600	50	Si	< 100	
Cr	6,3	0,8	Ti	< 1	
S	1421	70	V	< 2	
Na	512	12			
Fe	26	4			
			Particle size distribution determined by laser light diffraction method		
			D ₁₀	6,2 µm	0,5 µm
			D ₅₀	11,3 µm	0,5 µm
			D ₉₀	19,1 µm	1,2 µm
			Specific surface area (BET)		
				0,487 m ² /g	0,028 m ² /g

Graphite powder

BAM-S009 Medium purity graphite		
Certified values		
Parameter	Mass fraction in mg/kg	Uncertainty in mg/kg
Al	0,27	0,08
B	0,83	0,18
Ba	0,80	0,09
Be	0,00050	0,00027
Ca	5,1	1,1
Co	0,143	0,017
Cr	1,39	0,20
Cu	0,067	0,012
Fe	28	4
K	1,04	0,20
Li	0,022	0,007
Mg	0,135	0,030
Mn	0,094	0,015
Mo	0,20	0,04
Na	0,32	0,08
Ni	5,6	0,6
P	0,26	0,06
Pb	0,052	0,028
S	10,7	1,8
Si	41	6
Sr	0,32	0,05
Ti	8,6	1,6
V	1,30	0,17
W	3,0	0,6
Y	0,049	0,011
Zn	0,070	0,018
Zr	0,81	0,19
Values for information		
Parameter	Mass fraction in mg/kg	Uncertainty in mg/kg
Ag	0,0018	0,0010
As	0,016	0,007
Bi	0,016	0,012
Cd	0,0022	0,0019
Eu	0,0021	0,0010
Sb	0,022	0,015
Sc	0,012	0,010
Sn	0,16	0,05
Ta	0,018	0,014

BAM-S010 High purity graphite		
Certified values		
Parameter	Mass fraction in mg/kg	Uncertainty in mg/kg
Al	0,047	0,011
Ba	0,0023	0,0009
Be	0,000016	0,000008
Ca	0,061	0,029
Co	0,0008	0,0004
Cr	0,011	0,005
Cu	0,0049	0,0020
Fe	0,21	0,06
K	0,021	0,009
Li	0,00017	0,00010
Mg	0,019	0,005
Mn	0,0029	0,0008
Na	0,037	0,011
Ni	0,087	0,024
P	0,027	0,011
Pb	0,0029	0,0014
S	5,7	0,5
Sr	0,0008	0,0004
Ti	0,011	0,008
W	0,0036	0,0011
Y	0,00019	0,00010
Zn	0,014	0,008
Zr	0,0016	0,0005
Values for information		
Parameter	Mass fraction in mg/kg	Uncertainty in mg/kg
Ag	< 0,001	
As	0,0034	0,0008
B	0,0040	0,0019
Cd	0,00016	0,00009
Mo	0,0040	0,0019
Sb	< 0,03	
Si	0,27	0,09
Sn	< 0,02	
Te	< 0,002	
V	0,005	0,003

Multielement-glass

Mass fraction in mg/kg (bold in %)

		BAM-S005c		BAM-S006	
Element		Mass fraction ± uncertainty		Mass fraction ± uncertainty	
Al	(Al ₂ O ₃)	0,587 ± 0,018	(1,109)	1,081 ± 0,015	(2,042)
Ca	(CaO)	7,43 ± 0,12	(10,39)	7,660 ± 0,016	(10,72)
K	(K ₂ O)	0,595 ± 0,014	(0,717)	0,577 ± 0,008	(0,695)
Mg	(MgO)	1,37 ± 0,04	(2,28)	1,163 ± 0,010	(1,929)
Na	(Na ₂ O)	10,33 ± 0,24	(13,92)	8,79 ± 0,11	(11,85)
Si	(SiO ₂)	33,1 ± 0,5	(70,8)	33,10 ± 0,12	(70,83)
As	(As ₂ O ₃)	81 ± 4	(107)	9,0 ± 1,7	(11,8)
Ba	(BaO)	102 ± 4	(114)	456 ± 23	(509)
Cd	(CdO)	47 ± 4	(54)	0,24 ± 0,10	(0,27)
Ce	(CeO ₂)	80 ± 5	(98)	---	---
Co	(CoO)	33,2 ± 1,9	(42,3)	172 ± 5	(219)
Cr	(Cr ₂ O ₃)	10,8 ± 1,0	(15,8)	0,382 ± 0,008	(0,558)
Cu	(CuO)	86 ± 5	(107)	[26 ± 10]	(33)
Fe	(Fe ₂ O ₃)	295 ± 7	(422)	0,468 ± 0,008	(0,669)
Mn	(MnO)	69,6 ± 2,5	(89,9)	0,213 ± 0,004	(0,275)
Mo	(MoO ₃)	215 ± 7	(323)	---	---
Ni	(NiO)	41,3 ± 1,7	(52,6)	19,3 ± 1,4	(24,6)
P	(P ₂ O ₅)	---	---	85 ± 16	(195)
Pb	(PbO)	182 ± 8	(196)	103 ± 5	(111)
S	(SO ₃)	---	---	201 ± 10	(502)
Sb	(Sb ₂ O ₃)	103 ± 4	(123)	10,8 ± 1,5	(12,9)
Sn	(SnO ₂)	72,9 ± 2,3	(92,5)	---	---
Sr	(SrO)	134 ± 6	(158)	[130 ± 82]	(154)
Ti	(TiO ₂)	101 ± 6	(169)	388 ± 8	(647)
V	(V ₂ O ₅)	189 ± 8	(337)	---	---
Zn	(ZnO)	157 ± 6	(196)	[61 ± 7]	(76)
Zr	(ZrO ₂)	544 ± 26	(735)	[139 ± 28]	(188)
Cl		---	---	[180 ± 28]	

(Values in parenthesis are calculated using the molar masses)

[Values in paranthesis are for information only]

Iron in flat glass

BAM-S050, BAM-S051, BAM-S052

CRM	Parameter	Mass fraction in %	Uncertainty in %	Parameter	Mass fraction in %	Uncertainty in %
	Certified values				Values for information	
BAM-S050	Fe(II)	0,0026	0,0004	Fe(III), calculated	0,0058	0,0012
	Fe(total)	0,0084	0,0012	Fe(II), calculated as Fe ₂ O ₃	0,0037	0,0007
BAM-S051	Fe(II)	0,0155	0,0013	Fe(III), calculated	0,0326	0,0021
	Fe(total)	0,0481	0,0017	Fe(II), calculated as Fe ₂ O ₃	0,0226	0,0022
BAM-S052	Fe(II)	0,160	0,005	Fe(III), calculated	0,437	0,011
	Fe(total)	0,597	0,011	Fe(II), calculated as Fe ₂ O ₃	0,229	0,008

Borosilicate glass

BAM-S053

Hydrolytic resistance of borosilicate glass,
Glass grains tests (ISO 720, USP<660>, Ph.Eur. 3.2.1, ISO 719)

Acid consumption according to	Consumption of 0,02M HCl per g in mL	Uncertainty in mL
ISO 720	0,0422	0,0030
USP<660>	0,0428	0,0025
Ph.Eur. 3.2.1	0,0429	0,0026
	Values for information	
	Consumption of 0,01M HCl per g in mL	Uncertainty in mL
ISO 719	0,036	0,006

Acrylonitrile-butadiene-styrene copolymerisate (ABS)

BAM-H010

Analyte	Mass fraction $\mu\text{g/g}$	Uncertainty * $\mu\text{g/g}$
Pb	479	17
Br	240	21
Cd	93	5
Cr	470	36
Hg	(415)	—

(Value in parentheses an indicative value)

* The uncertainty is the expanded uncertainty with a coverage factor of $k=2$ and was determined according to the Guide to the Expression of Uncertainty in Measurement (GUM, ISO) 1993.

Pure substances

Mass fraction in µg/g (bold in %) ± 95%-confidence interval

CRM-No.	RS 1	RS 2	RS 3	RS 4	RS 5	RS 6A	RS 6B
Type	SiO ₂ ¹⁾ >99,99 %	Al ₂ O ₃ ²⁾ 99,76 %	CaCO ₃ ³⁾ 99,79 %	Ni ⁴⁾ 99,995 %	NiO ⁵⁾	MgO ⁶⁾ 100-350 µm	MgO ⁶⁾ 50-100 µm
Year	1991	1994	1994	1996	1996	1998	1998
CO ₂	–	–	43,95%	–	–	–	–
H ₂ O	–	0,22%	0,13%	–	0,015%	110	283
Ag	–	–	–	< 1	< 1	–	–
Al	8,7 ± 0,7	–	(< 5)	< 1	(< 15)	45 ± 9	49 ± 8
As	< 0,1	(< 0,5)	–	< 0,5	< 0,2	–	–
B	–	(< 5)	(< 0,2)	(< 2)	–	–	–
Ba	–	–	45,3 ± 1,7	–	< 1	(< 10)	(< 20)
Be	–	(< 0,2)	–	–	–	–	–
C	–	–	–	9,4 ± 2,0	14 ± 8	(< 50)	(< 210)
Ca	0,42 ± 0,09	3,1 ± 0,4	–	< 1	2,2 ± 0,9	994 ± 93	956 ± 149
Cd	< 0,05	(< 0,5)	(< 0,5)	< 0,2	< 0,2	–	–
Ce	–	(< 0,1)	–	–	–	–	–
Cl	–	(< 10)	–	–	–	–	–
Co	–	< 1	–	< 1	< 2	(< 5)	(< 5)
Cr	0,062 ± 0,021	< 1,5	< 1	< 0,5	16,1 ± 2,0	9,2	8,1
Cu	< 0,1	< 2,5	< 1	< 2	1,53 ± 0,18	(< 6)	(< 6)
Fe	0,62 ± 0,12	3,3 ± 1,6	< 5	4,2 ± 1,6	41 ± 7	72	71
Ga	–	(< 2)	(< 1,5)	< 0,2	< 0,5	–	–
Ge	< 1	–	–	–	–	–	–
Hg	< 0,05	–	–	(< 1)	–	–	–
In	–	(< 0,5)	–	(< 0,2)	(< 1)	–	–
K	0,48 ± 0,27	(< 5)	(< 30)	–	< 2	–	–
La	–	(< 0,3)	(< 0,5)	–	–	–	–
Li	0,25 ± 0,14	< 1	–	–	(< 2)	–	–
Mg	< 0,5	< 3	183 ± 5	< 0,8	< 1	60,19%	60,17%
Mn	< 0,2	< 1,5	3,0 ± 0,5	< 0,5	< 1	5,4	5,2
Mo	–	(< 1)	–	(< 0,2)	< 5	(< 10)	(< 10)
N	–	–	–	2,5 ± 1,0	–	–	–
Na	< 2	< 15	47,5 ± 2,7	(< 1)	< 2	–	–
Ni	< 0,2	< 10	(< 3)	99,995%±0,003%	78,57% ± 0,06%	3,9	3,3
O	–	–	–	(29)	21,41% ± 0,06%	–	–
Pb	< 0,15	–	(< 0,1)	< 1	< 2	(< 5)	(< 5)
S	–	–	–	(< 2)	(4)	–	–
Sb	–	–	–	< 0,2	(< 0,1)	–	–
Se	–	–	–	< 1	< 1	–	–
Si	–	< 20	(< 20)	(< 2)	(< 5)	–	–

(Values in parentheses are indicative values)

- continued -

Pure substances (continued)

CRM-No.	RS 1	RS 2	RS 3	RS 4	RS 5	RS 6A	RS 6B
Type	SiO ₂ ¹⁾ > 99,99 %	Al ₂ O ₃ ²⁾ 99,76 %	CaCO ₃ ³⁾ 99,79 %	Ni ⁴⁾ 99,995 %	NiO ⁵⁾	MgO ⁶⁾ 100-350 µm	MgO ⁶⁾ 50-100 µm
Year	1991	1994	1994	1996	1996	1998	1998
Sn	–	(< 1)	(< 1)	< 0,3	(< 1)	–	–
Sr	–	–	173 ± 8	–	(< 1)	2,0	2,1
Te	–	–	–	(< 0,2)	(< 0,2)	–	–
Ti	1,3 ± 0,4	< 2	(< 0,5)	–	(< 2)	1,3	1,2
Tl	–	–	–	< 0,2	(< 0,5)	–	–
V	–	(< 1)	–	(< 0,2)	< 1	8,4	7,8
W	–	–	–	(< 0,1)	(< 1)	–	–
Zn	< 1,3	< 2	< 2	< 4	3,4 ± 0,7	(< 6)	(< 6)
Zr	< 0,1	3,2 ± 1,3	(< 0,2)	–	(< 1)	(< 20)	(< 105)

(Values in parentheses are indicative values)

¹⁾ α-quartz, mean particle size: 150 µm

²⁾ α-aluminium oxide, average surface: 5,6 m²/g, bulk density: ca. 1,1 kg/L

³⁾ Pure calcite, the CO₂-content is given for the water free sample. It is 99,96 % of the theoretical value.

⁴⁾ Pure electrolytic nickel, the weight of one particle after milling is about 2 – 4 mg.

⁵⁾ Powdered nickel(II)oxide made by oxidation of powdered nickel (made by thermal decomposition of nickel carbonyl) with a particle size of 5 – 20 µm.

⁶⁾ Crystalline magnesium oxide with two different particle sizes

Platinum group elements (PGE) in used automobile catalyst

BAM-M504b[□]

Element	Certified value	Uncertainty
	Mass fraction in mg/kg	
Pt	1159	8
Pd	1128	9
Rh	314,2	2,6

[□] Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Electronic scrap

BAM-M505a

Element	Mass fraction in %	Uncertainty in %
Cu	16,76	0,04
Ni	0,694	0,006
Ag	0,0633	0,0009
Pb	1,13	0,05
Cr	0,980	0,017
Sn	0,468	0,015
	in mg/kg	in mg/kg
Au	52,4	0,9
Pd	48,0	0,8
Pt	5,7	0,4
As	372	20
Be	6,8	0,9
Cd	16,4	0,7
	Informative value	
	Mass fraction in mg/kg	Uncertainty in mg/kg
In	43	6
Hg	< 5	–

Environment

Calibration standards “Ethanol in Water” □

The certified reference materials are solutions of ethanol in water, prepared gravimetrically in units of about 4 L. The ethanol concentration at 20 °C is certified.

Application: Calibration of breath alcohol analysers according to DIN VDE 0405-4; validation of methods for the analysis of ethanol in aqueous samples

Identifier	Concentration g/L	Expanded Uncertainty g/L
BAM-K001	1,0292	± 0,0010
BAM-K002	0,0000	± 0,0001
BAM-K003	0,6100	± 0,0006
BAM-K004	1,2100	± 0,0012
BAM-K005	1,4500	± 0,0014
BAM-K006	1,8200	± 0,0018
BAM-K007	3,3900	± 0,0033

Currently, the calibration standards are only sold to customers in Germany. Certificates are only available in German. To customers outside of Germany the standards may be sold on request. Please pay attention to the delivery notes given in our webshop [<https://webshop.bam.de>]!

□ Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Calibration standard for the determination of mineral oil hydrocarbons in environmental matrices using gas chromatography

BAM-K010g □ Diesel oil/lubricating oil (1:1)

Certified parameter	Value in g/g	Uncertainty <i>U</i> in g/g
Mass ratio of diesel oil/lubricating oil	1,000028	0,000014
Mass fraction of the boiling range C ₁₀ – C ₄₀	0,969	0,015

BAM-K008a □ Diesel oil

Certified parameter	Value in g/g	Uncertainty <i>U</i> in g/g
Mass fraction of the boiling range C ₁₀ – C ₄₀	0,942	0,014

BAM-K009a □ Lubricating oil

Certified parameter	Value in g/g	Uncertainty <i>U</i> in g/g
Mass fraction of the boiling range C ₁₀ – C ₄₀	0,982	0,015

□ Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Sulfur in petrol

ERM®-EF213

This material is a petroleum product containing sulfur (S) in its natural forms, closely matching commercial petrol fuels at a sulfur concentration slightly lower than actual legal limits in Germany and EU. The absence of artificially added sulfur species avoids any effects arising from species specific analytical methods. A suitable supply of petrol was obtained in bulk from ESSO Deutschland GmbH, Ingolstadt, Germany. The main purpose of the materials is to assess method performance, i.e. for checking accuracy of analytical results. As any reference material, it can also be used for control charts or validation studies.

Certified property	Mass fraction	
	Certified value mg/kg	Uncertainty mg/kg
S	9,1	0,8

Adsorbed organically bound halogens (AOX) in soil

BAM-U024[□]

Measurand	Mass fraction mg/kg	Uncertainty mg/kg
AOX	42	2

Adsorbed organically bound halogens (AOX) in sludge

BAM-U025[□]

Measurand	Mass fraction mg/kg	Uncertainty mg/kg
AOX	253	11

[□] Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Mineral oil contaminated sediment and soil

BAM-U021a, BAM-U022, and BAM-U026

CRM-No.	Measurand	Certified value ¹⁾	Uncertainty ²⁾
BAM-U021a ^Δ soil	Total petrol hydrocarbon (TPH)	2801	204
BAM-U022 sediment	Total petrol hydrocarbon (TPH)	8270	550
BAM-U026 [□] soil	Total petrol hydrocarbon (TPH)	1355	130

All values are given in mg/kg.

¹⁾ Unweighted mean value of 11-14 laboratory means using gas chromatography with flame ionisation detection (GC/FID) according to ISO 16703:2005.

²⁾ Estimated expanded uncertainty with a coverage factor of $k = 2$, corresponding to a confidence level of approximately 95 %, as defined in the Guide to the Expression of Uncertainty in Measurement (GUM), ISO, 2008

^Δ Accredited by DAkkS as a producer of RM in accordance with ISO Guide 34 in combination with ISO/IEC 17025

[□] Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Polychlorinated biphenyls in soil

BAM-U019a^Δ

Measurand	Certifies values ¹⁾	Uncertainty ²⁾
PCB-28	0,157	0,021
PCB-52	1,67	0,23
PCB-101	1,8	0,4
PCB-118	1,48	0,16
PCB-138	1,02	0,13
PCB-153	0,84	0,19
PCB-180	0,213	0,030

All values are given in mg/kg.

¹⁾ Unweighted mean value of 10 laboratory means

²⁾ Estimated expanded uncertainty U with a coverage factor of $k = 2$, corresponding to a level of confidence of approx. 95 %, as defined in the Guide to the expression of uncertainty in measurement, (GUM, ISO/IEC Guide 98-3:2008) [1].

^Δ Accredited by DAkkS as a producer of RM in accordance with ISO Guide 34 in combination with ISO/IEC 17025

Pentachlorophenol (PCP) in wood

BAM-U030[□]

Measurand	Certifies value in mg/kg	Uncertainty ¹⁾ in mg/kg
Pentachlorophenol	7,19	0,80

¹⁾ Estimated expanded uncertainty U with a coverage factor of $k = 2$, corresponding to a level of confidence of approx. 95 %, as defined in the Guide to the expression of uncertainty in measurement, (GUM, ISO/IEC Guide 98-3:2008) [1].

[□] Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Trace elements in wood

BAM-U130

Element	Certifies value in mg/kg	Uncertainty ¹⁾ in mg/kg
As	4,0	0,4
Cd	2,52	0,30
Cr	39,3	2,7
Cu	30,0	2,7
Hg	0,66	0,06
Pb	41	5

¹⁾ Estimated expanded uncertainty U with a coverage factor of $k = 2$, corresponding to a level of confidence of approx. 95 %, as defined in the Guide to the expression of uncertainty in measurement, (GUM, ISO/IEC Guide 98-3:2008) [1].

Trace elements in contaminated river sediment

ERM®-CC020

CRM-No.	ERM®-CC020 River sediment	
Analyte	Aqua regia extractable mass fractions (ISO 11466)	
	Certified value	Uncertainty ¹⁾
As	56,6	2,6
Cd	20,8	0,5
Co	290	8
Cr	32,8	1,5
Cu	560	11
Hg	255	11
Ni	27,4	0,6
Pb	158	6
V	53	4
Zn	2030	40

All values are given in mg/kg.

¹⁾ Estimated expanded uncertainty with a coverage factor of $k=2,5$, corresponding to a level of confidence of about 95 %, as defined in the Guide to the Expression of Uncertainty in Measurement (GUM), ISO, 1995.

Total cyanide in soil

BAM-U117

Analyte	Certified value in mg/kg	Uncertainty in mg/kg
Total cyanide	11,0	0,7

Trace elements in sewage sludge ash

Iron rich sewage sludge ash

BAM-U200

Element	Total mass fractions		Aqua regia extractable mass fractions	
	Mass fraction in %	Uncertainty U in %	Mass fraction in %	Uncertainty U in %
Ca	13,2	2,1	13,1	2,1
Fe	10,0	1,0	9,9	0,9
P	8,8	1,3	7,9	1,4
Al	4,9	0,4	4,19	0,28
Mg	1,51	0,15	1,37	0,10
K	1,06	0,12	0,79	0,08
Na	0,51	0,10	0,32	0,06
Zn	0,270	0,016	0,235	0,018
Cu	0,131	0,008	0,114	0,029
	in mg/kg	in mg/kg	in mg/kg	in mg/kg
Pb	325	26	288	38
Cr	146	12	113	13
Ni	79	9	69	7
Sn	63	4	61	5
As	23,5	2,1	22,9	1,0
Cd	3,6	0,3	3,6	0,4

Aluminium rich sewage sludge ash

BAM-U201

Element	Total mass fractions		Aqua regia extractable mass fractions	
	Mass fraction in %	Uncertainty U in %	Mass fraction in %	Uncertainty U in %
Ca	11,5	1,7	11,2	1,1
Fe	12,8	1,1	11,2	0,6
P	8,42	1,03	7,72	0,60
Al	2,11	0,15	1,91	0,11
Mg	1,02	0,08	0,87	0,03
K	0,77	0,08	0,58	0,03
Na	0,46	0,10	0,30	0,05
Zn	0,25	0,02	0,22	0,01
Cu	0,12	0,01	0,11	0,01
	in mg/kg	in mg/kg	in mg/kg	in mg/kg
Pb	169,6	18,9	155,3	7,6
Cr	100,9	10,4	75,6	9,6
Ni	89,3	12,7	74,1	10,5
Sn	61,7	7	56,5	4
As	14,2	2,1	14,1	2,0
Cd	4,1	0,1	3,76	0,6

Food

Polycyclic aromatic hydrocarbons in olive oil

BAM-A001^Δ

Compound	Certified value	Uncertainty
Benz[a]anthracene	1,72 µg/kg	0,13 µg/kg
Chrysene	2,90 µg/kg	0,25 µg/kg
Benzo[b]fluoranthene	1,30 µg/kg	0,14 µg/kg
Benzo[a]pyrene	1,44 µg/kg	0,09 µg/kg

Acrylamide in crispbread

ERM®-BD272

Compound	Certified value	Uncertainty
Acrylamide	0,98 mg/kg	0,09 mg/kg

Acrylamide in rusk

ERM®-BD274

Compound	Certified value	Uncertainty
Acrylamide	74 µg/kg	7 µg/kg

Fusarium mycotoxins in wheat flour

ERM®-BC600

Compound ¹⁾	Certified value	Uncertainty
Deoxynivalenol (DON)	102 µg/kg	11 µg/kg
Nivalenol (NIV)	1000 µg/kg	130 µg/kg
Zearalenone (ZON)	90 µg/kg	8 µg/kg

¹⁾ DON, NIV and ZON as measured by using appropriate sample preparation techniques (e.g. solvent extraction, clean-up, derivatisation), instrumental separation (HPLC, GC) and detection techniques corrected for extraction efficiency/recovery.

Zearalenone in maize germ oil

ERM®-BC715^Δ

Compound	Certified value	Uncertainty
Zearalenone (ZON)	362 µg/kg	22 µg/kg

T-2 and HT-2 toxin in oat flakes

ERM®-BC720

Compound ¹⁾	Certified value	Uncertainty
T-2 toxin [CAS number: 21259-20-1]	82 µg/kg	4 µg/kg
HT-2 toxin [CAS number: 26934-87-2]	81 µg/kg	4 µg/kg

¹⁾ T-2 and HT-2 toxin measured using sample preparation, instrumental separation (HPLC) and mass spectrometric detection as specified on page 3 of the certificate.

Cadmium and Acrylamide in Cocoa

	Certified mass fraction of Cd in mg/kg	Uncertainty in mg/kg	Mass fraction of Acrylamide in mg/kg	Uncertainty in mg/kg
			(for information)	
ERM®-BD513	0,181	0,009	0,051	0,018
ERM®-BD514	0,541	0,024	0,101	0,026
ERM®-BD515	0,690	0,029	0,095	0,025

^Δ Accredited by DAkkS as a producer of RM in accordance with ISO/IEC 17034

Consumer products

Polycyclic aromatic hydrocarbons in rubber toy

BAM-B001[□]

Measurand ¹⁾	Mass fraction ²⁾ in mg kg ⁻¹	Uncertainty ³⁾ in mg kg ⁻¹
Fluorene	1,71	0,22
Phenanthrene	15,4	1,2
Anthracene	2,9	1,1
Fluoranthene	4,3	0,5
Pyrene	11,4	1,1
Benz[<i>a</i>]anthracene	2,17	0,22
Chrysene	2,08	0,15
Benzo[<i>b</i>]fluoranthene	0,57	0,05
Benzo[<i>k</i>]fluoranthene	0,213	0,022
Benzo[<i>j</i>]fluoranthene	0,40	0,04
Benzo[<i>e</i>]pyrene	1,21	0,16
Benzo[<i>a</i>]pyrene	1,41	0,10
Indeno[1,2,3- <i>cd</i>]pyrene	0,28	0,06
Benzo[<i>ghi</i>]perylene	1,43	0,09
Naphthalene	(0,09)	(0,08)
Acenaphthylene	(1,6)	(1,6)
Acenaphthene	(0,63)	(0,28)
Dibenz[<i>a,h</i>]anthracene	(0,118)	(0,020)

(Values in brackets are for information only)

[□] Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Gas mixtures

Certified reference gas mixtures

Certified reference gas mixtures (CRGM) are provided by BAM with compositions and expanded relative uncertainties ($k = 2$) according to GUM [1] as given in the tables below.

The customer has to provide the starting material and has to demonstrate that the starting material has been synthetically prepared according to ISO 6142 [2] or ISO 6144 [3].

The composition (i.e., amount of substance fractions of the specified analytes) of the starting material is certified with small uncertainty using a measurement procedure according to ISO 12963 [4] or ISO 6143 [5].

Certification of the starting material is carried out against primary standards prepared at BAM according to ISO 6142-1 [2]. By designation from PTB [6, 7], these primary standards are the National Standards of Germany for gas analysis, providing traceability to the International System of Units (SI).

The accordingly certified starting material becomes a measurement standard with transparent SI traceability.

Due to limited preparation capacity, BAM provides gas mixtures according to ISO 6142-1 [2] to customers only in exclusive cases and liable to charges.

Validity of the issued certificates is usually for a period of two years; exceptions apply for unstable mixtures.

Certified reference gas mixtures comprise:

1. Certified reference gas mixtures for vehicle exhaust emission measurements
 especially as defined in PTB-A 18.10 [10]
 especially as defined in [11]
 related to OIML [12]
2. Certified reference gas mixtures for energy gases
 especially as defined in PTB-A 7.63 [13]
3. Binary mixtures
4. Multicomponent certified reference gas mixtures

References:

[1] JCGM 100:2008 "Evaluation of measurement data – Guide to the expression of uncertainty in measurement" (GUM)

[2] ISO 6142-1:2015 "Gas analysis – Preparation of calibration gas mixtures – Part 1: Gravimetric method for Class I mixtures" or upcoming ISO 6142-2

[3] ISO 6144:2003 "Gas analysis – Preparation of calibration gas mixtures – Static volumetric method"

[4] ISO 12963:2017 "Gas analysis – Comparison methods for the determination of the composition of gas mixtures based on one- and two-point calibration"

[5] ISO 6143:2001 "Gas analysis – Comparison methods for determining and checking the composition of calibration gas mixtures"

[6] <https://www.bipm.org/en/about-us/member-states/de/cipm-mra.html> (accessed June 2020)

[7] PTB Physikalisch-Technische Bundesanstalt is the National Metrology Institute of Germany within the Metre Convention

[8] ISO/IEC 17025:2017 "General requirements for the competence of testing and calibration laboratories"

[9] ISO 17034:2016 "General requirements for the competence of reference material producers"

[10] PTB-Anforderung (Technical Requirement) PTB-A 18.10 „Messgeräte im Straßenverkehr; Abgasmessgeräte für Fremdzündungsmotoren“, PTB, January 2004, DOI: 10.7795/510.20150728T, Section 6.3.3

[11] Section 3.3.3.6 in „Richtlinie zur Kalibrierung von Abgasmessgeräten, die für die Untersuchung der Abgase von Kraftfahrzeugen nach Nummer 6.8.2 der Anlage VIIIa StVZO eingesetzt werden (AU-Geräte Kalibrierrichtlinie)“, rendered on 2018-05-23, Bundesministerium für Verkehr und digitale Infrastruktur, Verkehrsblatt Straßenverkehr Ausgabe Nr. 11/2018

- [12] International Recommendation OIML R 99-1 & 2 "Instruments for measuring vehicle exhaust emissions", International Organization of Legal Metrology (OIML), 2008, Annex B4 and others
- [13] PTB-Anforderung (Technical Requirement) PTB-A 7.63 „Messgeräte für Gas; Anforderungen an Kalibrier gas für Brennwert- und Gasbeschaffenheitsmessgeräte“, PTB, May 2011, DOI: 10.7795/510.20151109H, addendum published January 2018

Certified reference gas mixtures for vehicle exhaust emission measurements[□]

CRM-No.	Main component	Analyte	Amount of substance fraction cmol/mol	Relative expanded uncertainty %
BAM-G030-10+90 (PTB AU Q)	Nitrogen (N ₂)	Oxygen (O ₂)	10	0,5
BAM-G040-5+95 (PTB AU T)	Nitrogen (N ₂)	Carbon monoxide (CO)	5	0,5
BAM-G040-0,1+99,9 (PTB AU T1)	Nitrogen (N ₂)	Carbon monoxide (CO)	0,1	0,4
BAM-G040-0,01+99,99 (PTB AU T2)	Nitrogen (N ₂)	Carbon monoxide (CO)	0,01	0,6
BAM-G050-14+86 (PTB AU S)	Nitrogen (N ₂)	Carbon dioxide (CO ₂)	14	0,3
BAM-G070-0,2+99,8 (PTB AU N)	Nitrogen (N ₂)	Propane (C ₃ H ₈)	0,2	0,8
BAM-G070-0,02+99,98 (PTB AU M)	Nitrogen (N ₂)	Propane (C ₃ H ₈)	0,02	0,8
BAM-G100-0,1+99,9 (PTB AU P)	Nitrogen (N ₂)	Hexane (C ₆ H ₁₄)	0,1	0,3
BAM-G100-0,01+99,99 (PTB AU O)	Nitrogen (N ₂)	Hexane (C ₆ H ₁₄)	0,01	0,8
BAM-G200 (PTB AU IIA1)	Nitrogen (N ₂)	Carbon monoxide (CO)	2	0,5
BAM-G210 (PTB AU IIA2)	Nitrogen (N ₂)	Carbon monoxide (CO)	4,5	0,5
BAM-G220 (PTB AU IB)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈)	0,5 6 0,02	0,5 0,3 0,8
BAM-G221 (PTB AU E) (OIML E)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈) Oxygen (O ₂)	0,5 6 0,02 0,5	0,5 0,3 0,8 0,5
BAM-G225	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈)	1,5 11 0,06	0,5 0,3 0,5
BAM-G226 (PTB AU F) (OIML F)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈) Oxygen (O ₂)	1 10 0,06 10	0,5 0,3 0,5 0,5
BAM-G227 (PTB AU C)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈)	0,1 3 0,008	0,5 0,6 1,0
BAM-G230 (PTB AU D) (OIML D)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈)	3,5 14 0,2	0,5 0,3 0,5
BAM-G231 (PTB AU G)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈) Oxygen (O ₂)	3,5 14 0,2 20	0,5 0,3 0,5 0,5

□ Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Certified reference gas mixtures for vehicle exhaust emission measurements (continued) [□]

CRM-No.	Main component	Analyte	Amount of substance fraction cmol/mol	Relative expanded uncertainty %
BAM-G232 (PTB AU J) (OIML J)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈) Oxygen (O ₂)	3,5 14 0,2 10	0,3 0,3 0,5 0,5
BAM-G233 (PTB AU A) (OIML A)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈) Oxygen (O ₂)	0,5 14 0,02 0,5	0,5 0,3 0,8 0,5
BAM-G234 (PTB AU A1)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈) Oxygen (O ₂)	0,1 14 0,02 0,5	0,5 0,3 0,8 0,5
BAM-G235 (PTB AU K) (OIML K)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈) Hydrogen (H ₂)	3,5 14 0,2 5	0,5 0,3 0,5 0,5
BAM-G236 (PTB AU I) (OIML I)	Nitrogen (N ₂)	Carbon monoxide (CO) Propane (C ₃ H ₈)	3,5 0,2	0,5 0,5
BAM-G237 (PTB AU L)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈)	0,25 3 0,01	0,5 0,6 0,8
BAM-G238 (PTB AU B) (OIML B)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈)	0,5 14 0,02	0,5 0,3 0,8
BAM-G239 (PTB AU G1)	Nitrogen (N ₂)	Carbon dioxide (CO ₂) Propane (C ₃ H ₈) Oxygen (O ₂)	14 0,2 20,9	0,3 0,5 0,5
BAM-G240 (PTB AU H) (OIML H)	Nitrogen (N ₂)	Carbon monoxide (CO) Carbon dioxide (CO ₂) Propane (C ₃ H ₈) Oxygen (O ₂)	5 14 0,2 20,9	0,5 0,3 0,5 0,5

[□] Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Certified reference gas mixtures for energy gases

Certified reference gas mixtures for gas calorimeters[□]

CRM-No.	Main component	Analyte	Amount of substance fraction cmol/mol	Relative expanded uncertainty %
BAM-G300 (2H)	Methane (CH ₄)	Ethane (C ₂ H ₆)	12,3	0,3
BAM-G310 (2HL)	Methane (CH ₄)	Ethane (C ₂ H ₆)	6,5	0,3
BAM-G320 (2LH)	Methane (CH ₄)	Nitrogen (N ₂)	7	0,3
BAM-G330 (2LHL)	Methane (CH ₄)	Nitrogen (N ₂)	8,7	0,3
BAM-G340 (2L)	Methane (CH ₄)	Nitrogen (N ₂)	11,7	0,3
BAM-G350 (2LL)	Methane (CH ₄)	Nitrogen (N ₂)	17,5	0,3
BAM-G360 (3S)	Methane (CH ₄)	Nitrogen (N ₂)Hydrogen (H ₂)	17 49	0,3 0,5

(The "CRM-No." in parentheses corresponds to the name used in technical requirement "PTB-A 7.63" by PTB [13].)

□ Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Certified reference gas mixtures for process gas chromatographs[□]

CRM-No.	Main component	Analyte	Amount of substance fraction cmol/mol	Relative expanded uncertainty %
BAM-G400 (6H)	Methane (CH ₄)	Nitrogen (N ₂) Carbon dioxide (CO ₂) Ethane (C ₂ H ₆) Propane (C ₃ H ₈) n-Butane (C ₄ H ₁₀) Methane (CH ₄)	0,4 1,8 9,4 3,4 1 84	0,5 0,6 0,3 0,3 0,5 0,05
BAM-G401 (6L)	Methane (CH ₄)	Nitrogen (N ₂) Carbon dioxide (CO ₂) Ethane (C ₂ H ₆) Propane (C ₃ H ₈) n-Butane (C ₄ H ₁₀) Methane (CH ₄)	14,4 1 3 0,5 0,1 81	0,3 0,6 0,4 0,8 0,5 0,05
BAM-G410 (L1-8K)	Methane (CH ₄)	Nitrogen (N ₂) Carbon dioxide (CO ₂) Ethane (C ₂ H ₆) Propane (C ₃ H ₈) n-Butane (C ₄ H ₁₀) 2-Methyl-propane (C ₄ H ₁₀) 2-Methyl-butane (C ₅ H ₁₂) Methane (CH ₄)	12 4,5 0,75 0,3 0,2 0,2 0,05 82	0,3 0,6 0,8 0,8 0,5 0,5 0,5 0,05

(The "CRM-No." in parentheses corresponds to the name used in technical requirement "PTB-A 7.63" by PTB [13].)

□ Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Certified reference gas mixtures for process gas chromatographs (continued) [□]

CRM-No.	Main component	Analyte	Amount of substance fraction cmol/mol	Relative expanded uncertainty %
BAM-G411 (L2-8K)	Methane (CH ₄)	Nitrogen (N ₂)	10,3	0,3
		Carbon dioxide (CO ₂)	1	0,6
		Ethane (C ₂ H ₆)	4	0,4
		Propane (C ₃ H ₈)	1,25	0,4
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		Methane (CH ₄)	83	0,05
BAM-G412 (H1-8K)	Methane (CH ₄)	Nitrogen (N ₂)	1	0,5
		Carbon dioxide (CO ₂)	0,9	0,6
		Ethane (C ₂ H ₆)	1	0,4
		Propane (C ₃ H ₈)	0,25	0,8
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		Methane (CH ₄)	96,4	0,05
BAM-G413 (H2-8K)	Methane (CH ₄)	Nitrogen (N ₂)	4	0,3
		Carbon dioxide (CO ₂)	1,5	0,6
		Ethane (C ₂ H ₆)	8,2	0,4
		Propane (C ₃ H ₈)	2	0,3
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		Methane (CH ₄)	83,85	0,05
BAM-G420 (11M)	Methane (CH ₄)	Oxygen (O ₂)	0,5	0,5
		Nitrogen (N ₂)	4	0,3
		Carbon dioxide (CO ₂)	1,5	0,6
		Ethane (C ₂ H ₆)	4	0,4
		Propane (C ₃ H ₈)	1	0,4
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,05	0,5
		Methane (CH ₄)	88,45	0,05
BAM-G422 (P1-11K)	Methane (CH ₄)	Nitrogen (N ₂)	8	0,3
		Carbon dioxide (CO ₂)	3	0,6
		Ethane (C ₂ H ₆)	6,5	0,3
		Propane (C ₃ H ₈)	2	0,3
		n-Butane (C ₄ H ₁₀)	0,5	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,5	0,5
		n-Pentane (C ₅ H ₁₂)	0,1	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,1	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,025	0,8
		n-Hexane (C ₆ H ₁₄)	0,025	0,8
		Methane (CH ₄)	79,25	0,05

(The "CRM-No." in parentheses corresponds to the name used in technical requirement "PTB-A 7.63" by PTB [13].)

□ Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Certified reference gas mixtures for process gas chromatographs (continued) [□]

CRM-No.	Main component	Analyte	Amount of substance fraction cmol/mol	Relative expanded uncertainty %
BAM-G430 (11D)	Methane (CH ₄)	Nitrogen (N ₂)	4	0,3
		Carbon dioxide (CO ₂)	1,5	0,6
		Ethane (C ₂ H ₆)	4	0,4
		Propane (C ₃ H ₈)	1	0,4
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,05	0,5
		Methane (CH ₄)	88,9	0,05
BAM-G431 (H1-11K)	Methane (CH ₄)	Nitrogen (N ₂)	1,35	0,4
		Carbon dioxide (CO ₂)	0,35	0,6
		Ethane (C ₂ H ₆)	0,4	0,8
		Propane (C ₃ H ₈)	0,2	0,8
		n-Butane (C ₄ H ₁₀)	0,1	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,1	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,05	0,5
		Methane (CH ₄)	97,3	0,05
BAM-G432 (H2-11K)	Methane (CH ₄)	Nitrogen (N ₂)	0,95	0,5
		Carbon dioxide (CO ₂)	1,45	0,6
		Ethane (C ₂ H ₆)	9	0,3
		Propane (C ₃ H ₈)	3	0,3
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,05	0,5
		Methane (CH ₄)	85	0,05
BAM-G433 (H3-11K)	Methane (CH ₄)	Nitrogen (N ₂)	2,5	0,3
		Carbon dioxide (CO ₂)	1	0,6
		Ethane (C ₂ H ₆)	6,5	0,3
		Propane (C ₃ H ₈)	1,3	0,4
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,25	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,025	0,8
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,05	0,5
		Methane (CH ₄)	88,075	0,05
BAM-G434 (L1-11K)	Methane (CH ₄)	Nitrogen (N ₂)	11	0,3
		Carbon dioxide (CO ₂)	1,55	0,6
		Ethane (C ₂ H ₆)	0,75	0,8
		Propane (C ₃ H ₈)	0,3	0,8
		n-Butane (C ₄ H ₁₀)	0,1	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,1	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,05	0,5
		Methane (CH ₄)	86	0,05

(The "CRM-No." in parentheses corresponds to the name used in technical requirement "PTB-A 7.63" by PTB [13].)

[□] Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Certified reference gas mixtures for process gas chromatographs (continued) [□]

CRM-No.	Main component	Analyte	Amount of substance fraction cmol/mol	Relative expanded uncertainty %
BAM-G435	Methane (CH ₄)	Nitrogen (N ₂)	1,2	0,5
		Carbon dioxide (CO ₂)	0,8	0,6
		Ethane (C ₂ H ₆)	11	0,3
		Propane (C ₃ H ₈)	4,5	0,3
		n-Butane (C ₄ H ₁₀)	0,1	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,1	0,5
		n-Pentane (C ₅ H ₁₂)	0,035	0,8
		2-Methyl-butane (C ₅ H ₁₂)	0,035	0,8
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,02	0,8
		Methane (CH ₄)	82,16	0,05
BAM-G436 (L2-11K)	Methane (CH ₄)	Nitrogen (N ₂)	9,2	0,3
		Carbon dioxide (CO ₂)	1,8	0,6
		Ethane (C ₂ H ₆)	3	0,4
		Propane (C ₃ H ₈)	0,5	0,8
		n-Butane (C ₄ H ₁₀)	0,1	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,1	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,05	0,5
		Methane (CH ₄)	85,1	0,05
BAM-G437	Methane (CH ₄)	Nitrogen (N ₂)	0,8	0,5
		Carbon dioxide (CO ₂)	1	0,6
		Ethane (C ₂ H ₆)	1	0,8
		Propane (C ₃ H ₈)	0,5	0,8
		n-Butane (C ₄ H ₁₀)	0,1	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,1	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,1	0,5
		Methane (CH ₄)	96,25	0,05
BAM-G440 (16M)	Methane (CH ₄)	Helium (He)	0,5	1,0
		Oxygen (O ₂)	0,5	0,5
		Nitrogen (N ₂)	5	0,3
		Carbon dioxide (CO ₂)	1	0,6
		Carbon monoxide (CO)	0,5	0,5
		Hydrogen (H ₂)	1	0,8
		Ethene (C ₂ H ₄)	0,5	0,8
		Ethane (C ₂ H ₆)	2,5	0,4
		Propene (C ₃ H ₆)	0,5	0,8
		Propane (C ₃ H ₈)	1	0,5
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,06	0,5
		Methane (CH ₄)	86,44	0,05

(The "CRM-No." in parentheses corresponds to the name used in technical requirement "PTB-A 7.63" by PTB [13].)

[□] Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Certified reference gas mixtures for process gas chromatographs (continued) [□]

CRM-No.	Main component	Analyte	Amount of substance fraction cmol/mol	Relative expanded uncertainty %
BAM-G441 (12M)	Methane (CH ₄)	Oxygen (O ₂)	0,5	0,5
		Nitrogen (N ₂)	4	0,3
		Carbon dioxide (CO ₂)	1,5	0,6
		Hydrogen (H ₂)	1	0,8
		Ethane (C ₂ H ₆)	4	0,4
		Propane (C ₃ H ₈)	1	0,5
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,05	0,5
		Methane (CH ₄)	87,45	0,05
BAM-G442 (13K)	Methane (CH ₄)	Oxygen (O ₂)	0,5	0,5
		Nitrogen (N ₂)	4	0,3
		Carbon dioxide (CO ₂)	1,5	0,6
		Hydrogen (H ₂)	1	0,8
		Ethane (C ₂ H ₆)	4	0,4
		Propane (C ₃ H ₈)	1	0,5
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,05	0,5
		Methane (CH ₄)	87,40	0,05
BAM-G443 (P1-13K)	Methane (CH ₄)	Helium (He)	0,25	1,0
		Oxygen (O ₂)	0,3	0,5
		Nitrogen (N ₂)	4	0,3
		Carbon dioxide (CO ₂)	4	0,6
		Hydrogen (H ₂)	7	0,5
		Ethane (C ₂ H ₆)	5,5	0,3
		Propane (C ₃ H ₈)	2	0,3
		n-Butane (C ₄ H ₁₀)	0,5	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,3	0,5
		n-Pentane (C ₅ H ₁₂)	0,1	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,1	0,5
		n-Hexane (C ₆ H ₁₄)	0,06	0,8
		Methane (CH ₄)	75,89	0,05
BAM-G444 (P-3K)	Methane (CH ₄)	Nitrogen (N ₂)	3	0,3
		Hydrogen (H ₂)	4,5	0,5
		Methane (CH ₄)	92,5	0,05
BAM-G446 (B-5K)	Methane (CH ₄)	Oxygen (O ₂)	1	0,5
		Nitrogen (N ₂)	2	0,3
		Carbon dioxide (CO ₂)	5,5	0,6
		Hydrogen (H ₂)	2	0,8
		Methane (CH ₄)	89,5	0,05
BAM-G449 (B3-5K)	Methane (CH ₄)	Oxygen (O ₂)	1	0,5
		Nitrogen (N ₂)	18	0,3
		Carbon dioxide (CO ₂)	2,5	0,6
		Hydrogen (H ₂)	15	0,5
		Methane (CH ₄)	63,5	0,07

(The "CRM-No." in parentheses corresponds to the name used in technical requirement "PTB-A 7.63" by PTB [13].)

[□] Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Certified reference gas mixtures for process gas chromatographs (continued) [□]

CRM-No.	Main component	Analyte	Amount of substance fraction cmol/mol	Relative expanded uncertainty %
BAM-G450 (17K)	Methane (CH ₄)	Helium (He)	0,5	1,0
		Oxygen (O ₂)	0,5	0,5
		Nitrogen (N ₂)	5	0,3
		Carbon dioxide (CO ₂)	1	0,6
		Carbon monoxide (CO)	0,5	0,5
		Hydrogen (H ₂)	1	0,8
		Ethene (C ₂ H ₄)	0,5	0,8
		Ethane (C ₂ H ₆)	2,5	0,4
		Propene (C ₃ H ₆)	0,5	0,8
		Propane (C ₃ H ₈)	1	0,5
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,06	0,5
		Methane (CH ₄)	86,39	0,05
BAM-G451	Methane (CH ₄)	n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,05	0,5
		Methane (CH ₄)	99,80	0,05
BAM-G452	Methane (CH ₄)	Helium (He)	0,5	1,0
		Nitrogen (N ₂)	12	0,3
		Carbon dioxide (CO ₂)	4	0,6
		Hydrogen (H ₂)	3	0,5
		Ethane (C ₂ H ₆)	0,75	0,8
		Propane (C ₃ H ₈)	0,3	0,8
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,05	0,5
		Methane (CH ₄)	78,85	0,05
BAM-G460	Methane (CH ₄)	Helium (He)	0,5	1,0
		Nitrogen (N ₂)	12	0,3
		Carbon dioxide (CO ₂)	4	0,6
		Ethane (C ₂ H ₆)	0,75	0,8
		Propane (C ₃ H ₈)	0,3	0,8
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		n-Pentane (C ₅ H ₁₂)	0,05	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,05	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,05	0,5
		n-Hexane (C ₆ H ₁₄)	0,05	0,5
		Methane (CH ₄)	81,85	0,05

(The "CRM-No." in parentheses corresponds to the name used in technical requirement "PTB-A 7.63" by PTB [13].)

[□] Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Certified reference gas mixtures for process gas chromatographs (continued) [□]

CRM-No.	Main component	Analyte	Amount of substance fraction cmol/mol	Relative expanded uncertainty %
BAM-G471 (9M)	Methane (CH ₄)	Oxygen (O ₂)	0,4	0,5
		Nitrogen (N ₂)	4	0,3
		Carbon dioxide (CO ₂)	2,5	0,6
		Hydrogen (H ₂)	0,2	1,0
		Ethane (C ₂ H ₆)	2,5	0,3
		Propane (C ₃ H ₈)	1	0,5
		n-Butane (C ₄ H ₁₀)	0,2	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,2	0,5
		Methane (CH ₄)	89	0,05
BAM-G472 (9E)	Methane (CH ₄)	Oxygen (O ₂)	2	0,3
		Nitrogen (N ₂)	8	0,3
		Carbon dioxide (CO ₂)	2	0,6
		Hydrogen (H ₂)	1	0,8
		Ethane (C ₂ H ₆)	4	0,4
		Propane (C ₃ H ₈)	3	0,3
		n-Butane (C ₄ H ₁₀)	0,5	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,5	0,5
		Methane (CH ₄)	79	0,05
BAM-G473 (P1-9K)	Methane (CH ₄)	Oxygen (O ₂)	0,3	0,5
		Nitrogen (N ₂)	3	0,3
		Carbon dioxide (CO ₂)	3,5	0,6
		Hydrogen (H ₂)	0,3	1,0
		Ethane (C ₂ H ₆)	0,35	0,8
		Propane (C ₃ H ₈)	4,75	0,3
		n-Butane (C ₄ H ₁₀)	0,3	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,3	0,5
		Methane (CH ₄)	87,2	0,05
BAM-G474	Methane (CH ₄)	Nitrogen (N ₂)	0,12	0,5
		Carbon dioxide (CO ₂)	0,02	0,6
		Ethane (C ₂ H ₆)	10	0,3
		Propane (C ₃ H ₈)	2	0,3
		n-Butane (C ₄ H ₁₀)	0,15	0,5
		2-Methyl-propane (C ₄ H ₁₀)	0,15	0,5
		n-Pentane (C ₅ H ₁₂)	0,02	0,8
		2-Methyl-butane (C ₅ H ₁₂)	0,02	0,8
		Methane (CH ₄)	87,52	0,05
BAM-G494	Methane (CH ₄)	Nitrogen (N ₂)	4	0,3
		Carbon dioxide (CO ₂)	1,5	0,6
		n-Butane (C ₄ H ₁₀)	3	0,5
		n-Pentane (C ₅ H ₁₂)	0,3	0,5
		2-Methyl-butane (C ₅ H ₁₂)	0,3	0,5
		2,2-Dimethyl-propane (C ₅ H ₁₂)	0,3	0,5
		n-Hexane (C ₆ H ₁₄)	0,3	0,5
		Methane (CH ₄)	90,3	0,05
BAM-G901	Natural gas	Carbon dioxide (CO ₂)	0,2 to 20	0,5 to 0,3

(The "CRM-No." in parentheses corresponds to the name used in technical requirement "PTB-A 7.63" by PTB [13].)

[□] Accredited by DAkkS as a producer of RM in accordance with ISO 17034

Binary certified reference gas mixtures

CRM-No.	Main component	Analyte	Range of amount of substance fraction cmol/mol	Range of relative expanded uncertainty %
BAM-G010	Nitrogen (N ₂)	Helium (He)	1 to 50	0,8 to 0,5
BAM-G012	Synth. air	Helium (He)	0,5 to 50	2,0 to 0,5
BAM-G014	Argon (Ar)	Helium (He)	1 to 50	0,5
BAM-G020	Nitrogen (N ₂)	Hydrogen (H ₂)	1 to 20	0,8 to 0,5
BAM-G022	Helium (He)	Hydrogen (H ₂)	0,1 to 20	1,0 to 0,3
BAM-G024	Argon (Ar)	Nitrogen (N ₂)	1 to 50	0,5
BAM-G025-0,1+99,9	Methane (CH ₄)	Hydrogen (H ₂)	0,1	0,5
BAM-G030	Nitrogen (N ₂)	Oxygen (O ₂)	1 to 20	0,5
BAM-G037	Helium (He)	Nitrogen (N ₂)	0,001 to 0,1	1,0 to 0,5
BAM-G038	Helium (He)	Argon (Ar)	0,0005 to 0,2	1,0 to 0,3
BAM-G039	Helium (He)	Oxygen (O ₂)	1 to 20	1,0 to 0,5
BAM-G040	Nitrogen (N ₂)	Carbon monoxide (CO)	0,001 to 10	1,0 to 0,3
BAM-G042	Synth. air	Carbon monoxide (CO)	0,01 to 1	1,0 to 0,5
BAM-G050	Nitrogen (N ₂)	Carbon dioxide (CO ₂)	0,001 to 50	0,5 to 0,3
BAM-G052	Synth. air	Carbon dioxide (CO ₂)	0,01 to 20	1,0 to 0,3
BAM-G055	Methane (CH ₄)	Carbon dioxide (CO ₂)	0,5 to 10	0,5
BAM-G060	Nitrogen (N ₂)	Methane (CH ₄)	0,001 to 50	1,0 to 0,3
BAM-G062	Synth. air	Methane (CH ₄)	0,01 to 0,1	1,0 to 0,5
BAM-G070	Nitrogen (N ₂)	Propane (C ₃ H ₈)	0,005 to 1	1,0 to 0,5
BAM-G072	Synth. air	Propane (C ₃ H ₈)	0,01 to 0,1	1,0 to 0,5
BAM-G100	Nitrogen (N ₂)	n-Hexane (C ₆ H ₁₄)	0,01 to 0,1	0,8 to 0,3

For binary certified reference gas mixtures only a limited amount of calibration gases is actually on stock. Hence, certification of starting materials with specific values for the amount of substance fraction might require additional time.

Multicomponent certified reference gas mixtures

CRM-No.	Main component	Analyte	Amount of substance fraction cmol/mol	Relative expanded uncertainty %
BAM-G501	Nitrogen (N ₂)	Oxygen (O ₂) Argon (Ar)	20 1	0,5 0,5
BAM-G510	Nitrogen (N ₂)	Carbon monoxide (CO) Methane (CH ₄)	0,3 0,3	0,5 0,5
BAM-G530	Nitrogen (N ₂)	Oxygen (O ₂) Hydrogen (H ₂)	1,5 10	0,5 0,5

Elastomeric materials

Standard reference elastomers (SRE) from vulcanized rubbers

Standard Reference Elastomers (SRE) are characterized by standardized and controlled properties. One application area is the calibration of scientific and technical test apparatuses and methods (E001 and E003). They enable the exact determination of material data if the method of measuring by itself cannot give absolute measured values. They can further be used as part of a measuring device (E002, E004 to E007). The SRE E001, E003 to E007 consist of natural rubber (NR).

SRE made from nitrile rubber (NBR), hydrogenated nitrile rubber (HNBR), ethylene-propylene diene rubber (EPDM), polyacrylate rubber (ACM), silicone rubber (MVQ), fluoropolymer rubber (FKM) and chloroprene rubber (CR) are meant to determine the effect of mineral oils, lubricants, hydraulic liquids and other service fluids on vulcanizates made from the mentioned rubbers which are used for seals, hoses etc. They are different in their degree of swelling (E008 to E021). In most cases the physical properties of the elastomers such as density, hardness, compression set and tensile stress-strain are also specified.

The following SRE from vulcanized rubbers and for testing of vulcanized rubber products (E002) are produced and offered:

BAM-E001	Rubber test sheet for determination of abrasion resistance of vulcanized rubber according to DIN 53516 and ISO 4649 standard reference compound no. 1
BAM-E002	Abrasive paper sheet - according to DIN 53516 and ISO 4649; Annex A
BAM-E003	Rubber test sheet for determination of abrasion resistance of vulcanized rubber according to ISO 4649 standard reference compound no. 2
BAM-E004	Rubber sole sheet for measuring the electrostatic charging of floor by a walking test
BAM-E005	Rubber base ring for the portable tester for measuring the surface roughness of streets (Efflux meter in accordance with MOORE) according to EN 13036-3
BAM-E006/ BAM-E007	Rubber slider for the pendulum tester for measuring the surface grip property of streets (skid resistance test; SRT) according to EN 13036-4: 2003; CEN rubber and for the pendulum tester for the determination of the PSV-value (polished stone value) according to EN 1097-8
BAM-E008	Elastomer ISO 13226 SRE-NBR 28/PX designated for hydraulic area (vulcanized with peroxide, low elongation at break)
BAM-E009	Elastomer ISO 13226 SRE-NBR 28/SX designated for automotive area (vulcanized with thiurame, high elongation at break)
BAM-E010	Elastomer ISO 13226 SRE-NBR 34/SX designated for automotive area (vulcanized with thiurame, high elongation at break)
BAM-E011	Elastomer ISO 13226 SRE-HNBR/1X designated for hydraulic and automotive area (vulcanized with peroxide)
BAM-E012	Elastomer ISO 13226 SRE-ACM/1X designated for hydraulic and automotive area
BAM-E013	Elastomer ISO 13226 SRE-VMQ/1X designated for hydraulic and automotive area (vulcanized with peroxide)
BAM-E014	Elastomer ISO 13226 SRE-FKM/2X / ISO 6072 FKM 2 designated for hydraulic and automotive area
BAM-E015	Elastomer ISO 6072 NBR 1 designated for hydraulic and automotive area
BAM-E016	Elastomer ISO 6072 NBR 2 designated for hydraulic and automotive area
BAM-E017	Elastomer ISO 13226 SRE-NBR L designated for hydraulic and automotive area (vulcanized with thiurame, low content of acrylonitrile)
BAM-E018	Elastomer ISO 13226 SRE-NBR M designated for hydraulic and automotive area (vulcanized with thiurame, medium content of acrylonitrile)
BAM-E019	Elastomer ISO 6072 EPDM 1 designated for hydraulic and automotive area
BAM-E020	Elastomer ISO 6072 HNBR 1 designated for hydraulic and automotive area
BAM-E021	Elastomer ISO 13226 SRE-CR/1 designated for hydraulic and automotive area

BAM-E022	Rubber Slider for the pendulum tester (Skid Resistance Test, SRT) according to EN 13036-4: 2011; slider 57
BAM-E023	Rubber Slider Pad for the pendulum tester (SRT) according to EN 13036-4:2003; CEN rubber
BAM-E024	Rubber Slider Pad for the pendulum tester (SRT) according to EN 13036-4:2011; slider 57
BAM-E025	Reference Material for the determination of rebound resilience according to ISO 4662
BAM-E027	Rubber Slider for the pendulum tester according to EN 1338:2003/AC:2006, annex I

In addition to the described applications, these SRE can generally be used in all cases in which elastomers with defined and reproducible properties are needed.

Optical properties

X-ray film step tablet

BAM-X001

Calibrated X-ray film step tablet of 15 steps

Covered optical density range: 0,25 – 5,0

Film type: Agfa - Gevaert Structurix D4

Calibration kit Spectral fluorescence standards


BAM-FCalKit

Five spectral fluorescence standards BAM-F001b, BAM-F002b, BAM-F003b, BAM-F004b, BAM-F005b which cover the spectral region of 300 nm to 760 nm as a set.

For the determination of the relative spectral responsivity of fluorescence instruments using the CRM data and the evaluation software LINKCORRWin1.3, the control of the long-term stability of fluorescence instruments, and for the determination of corrected, i.e., instrument-independent emission spectra.

Certified properties

Normalized corrected fluorescence emission spectra of BAM-F001b – BAM-F005b in ethanol for $T = 25\text{ °C}$. The emission spectra are traceable to the spectral photon radiance scale realized and disseminated in Germany by the Physikalisch-Technische Bundesanstalt (PTB) Berlin.

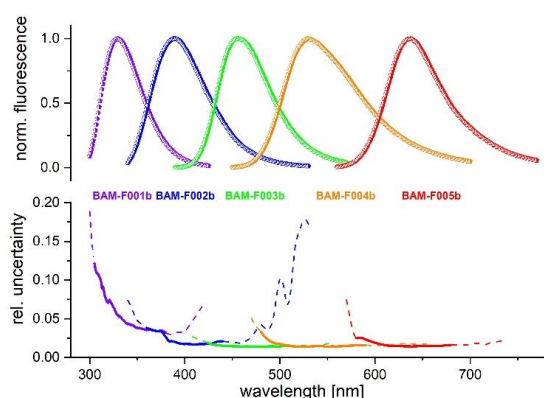

Certified normalized corrected
fluorescence emission spectra of

← BAM-F001b – BAM-F005b

and

← expanded relative uncertainties

Fluorescence Quantum Yield Standards

Product	Excitation wavelength range	Fluorescence wavelength range	Product	Excitation wavelength range	Fluorescence wavelength range
BAM-F019	335 nm – 390 nm	415 nm – 610 nm	BAM-F020	510 nm – 700 nm	540 nm – 735 nm
BAM-F016	365 nm – 435 nm	460 nm – 775 nm	BAM-F022	465 nm – 620 nm	680 nm – 1100 nm
BAM-F018	415 nm – 490 nm	525 nm – 800 nm	BAM-F023	480 nm – 635 nm	670 nm – 1000 nm
BAM-F011	460 nm – 510 nm	490 nm – 650 nm	BAM-F021	575 nm – 650 nm	620 nm – 860 nm
BAM-F015	485 nm – 535 nm	510 nm – 655 nm	BAM-F014	650 nm – 745 nm	685 nm – 1005 nm
BAM-F017	470 nm – 565 nm	565 nm – 800 nm	BAM-F013	690 nm – 795 nm	750 nm – 1010 nm

Solid in a tightly closed glass bottle, <1 mg for direct solution with different solvents directly before use.

Porous reference materials

CRMs for the gas adsorption method

CRM-No.	BAM-PM-101	BAM-PM-102	ERM®-FD107	BAM-P109
Description	SiO ₂ Powder	alpha-Al ₂ O ₃ Powder	Faujasite type zeolite Pellets	Nanoporous carbon Beads
Adsorptive	Krypton	Nitrogen	Nitrogen	Nitrogen
Year of issue	1996	1996	2000	2010
BET Specific surface area (m ² /g)	0,177 ± 0,014	5,41 ± 0,24	–	1396 ± 24
Specific pore volume (cm ³ /g) <i>p/p₀</i> =0,99	–	–	–	–
Mean pore diameter (nm)	–	–	–	–
Most frequent pore diameter (nm)	–	–	–	–
Specific micropore volume (cm ³ /g)	–	–	0,217 ± 0,002	–
Median pore width (nm)	–	–	0,86 ± 0,02	–

CRM-No.	BAM-P110	BAM-P114	BAM-P115 [□]	BAM-P116 [□]
Description	Titanium dioxide (Anatase)	Titanium dioxide (Anatase/Rutile)	Titanium dioxide (Anatase/Rutile)	Titanium dioxide (Anatase)
Adsorptive	Nitrogen	Nitrogen	Nitrogen	Nitrogen
Year of issue	2016	2021	2020	2020
BET Specific surface area (m ² /g)	107,8 ± 1,6	24,48 ± 0,30	147,3 ± 2,8	325 ± 11
Specific pore volume (cm ³ /g) <i>p/p₀</i> =0,99	–	–	0,214 ± 0,004	–
Hydraulic pore diameter (nm)	–	–	5,79 ± 0,07	–
Modal pore diameter (des. in nm)	–	–	4,75 ± 0,21	–
Modal pore diameter (abs. in nm)	–	–	5,40 ± 0,24	–
Specific micropore volume (cm ³ /g)	–	–	–	–
Median pore width (nm)	–	–	–	–

¹⁾ calculated from the desorption branch of the isotherm

²⁾ calculated from the adsorption branch of the isotherm

Note: The uncertainty given here is ± 1 s (standard deviation of the laboratory means) for BAM-PM-101 to 102. In the case of BAM-P109 to 116 and ERM®-FD107 it is the expanded uncertainty with a coverage factor of *k*=2.

The reference materials are intended for checking the performance of instruments used for the determination of BET specific surface area, specific pore volume, and the pore diameter (pore width) by means of the gas adsorption methods according to DIN 66131 (replaced by DIN ISO 9277), DIN 66134, DIN 66135-4, ISO 9277, ISO 15901-2 and ISO 15901-3.

□ Accredited by DAkkS as a producer of RM according to ISO 17034

CRMs for the mercury intrusion method

High pressure range between 0,1 and 400 MPa

Certified properties:

- A) Pressure-volume curve (mercury intrusion curve) between 0,1 MPa and 400 MPa
 B) Diameter-volume curve (cumulative pore volume curve) between 3,7 nm and 14708 nm (for A and B see certificate)
 C) (i) Pore volume values at selected intrusion pressure points;
 (ii) Values for the pore diameter (see the table below)

CRM-No.	ERM®-FD120 (BAM-PM-120)	ERM®-FD122 (BAM-PM-122)	BAM-P127*
Description	alpha-Alumina	Porous glass	Alumina
	Beads	Beads	Beads
Year of issue	2000	2000	2002
Pore volume (in mm ³ /g) at 50 MPa	–	–	69,4 ± 8,0
Pore volume (in mm ³ /g) at 100 MPa	545,0 ± 12,2	919,7 ± 16,8	625,4 ± 13,6
Pore volume (in mm ³ /g) at 195 MPa	546,7 ± 12,7	922,5 ± 17,5	637,1 ± 14,4
Pore volume (in mm ³ /g) at 200 MPa	546,8 ± 12,7	922,6 ± 17,5	–
Pore volume (in mm ³ /g) at 395 MPa	548,1 ± 13,1	924,4 ± 17,2	638,6 ± 21,6
Mean pore diameter d_{50} (nm)	228,0 ± 5,9	139,0 ± 3,7	24,2 ± 1,0
Most frequent pore diameter $d_{p,m}$ (nm)	232,2 ± 8,8	140,2 ± 3,9	23,9 ± 2,8

* 1st CRM jointly developed by NIST and BAM (identical with NIST SRM 1917)

Note: All certified pore volumes are normalized values $V'_p = V_p(p_{Hg}) - V_p(0,1 \text{ MPa})$

The uncertainty is the expanded uncertainty for the selected intrusion pressure points for ERM®-FD120, ERM®-FD121, ERM®-FD122 and for BAM-P127
 These reference materials are intended for the calibration and checking of porosimeters by means of the whole pressure volume curves of the Hg intrusion method.

ERM®-FD123

Mercury intrusion curve between 0,28 MPa and 1,41 MPa

Ceramic filter tubes

Pressure-volume curve characteristics

Quantity	Certified value ¹⁾	Uncertainty ²⁾	Unit
y_1 ³⁾	99,52	3,44	mm ³ g ⁻¹
y_2 ⁴⁾	0,4966	0,0180	MPa
y_3 ⁵⁾	0,2151	0,0156	MPa
p_{50}	0,4829	0,0239	MPa
d_{50}	3,0520	0,1533	µm

¹⁾ Pressure volume curves from designed round robins are analysed by means of a multivariate variance components model for the curves characteristics y_1 , y_2 and y_3 . The results are mean curve characteristics (certified values) and confidence intervals for the curve characteristics. Adjusted curves and statistics from the variance components model are used to create a certified pressure volume curve with confidence bands and prediction bands.

²⁾ Half-width of the confidence interval resulting from the variance analytical investigation of the pressure volume curve characteristics y_1 , y_2 , and y_3 at the significance level 0,95.

³⁾ y_1 : Intruded volume at the saturation point 1,41 MPa (saturation value).

⁴⁾ y_2 : Pressure at 57,5 % of the saturation value. This value has been determined by local polynomial estimation (Epanechnikov kernel with band width $h = 0,035 \text{ MPa}$).

⁵⁾ y_3 : Difference of the pressures at which the intrusion curve has got 87,5 % and 25 % respectively of the saturation value.

BAM-P124**Mercury intrusion curve between 0,24 MPa and 1,55 MPa**

Flat membrane

Mercury intrusion curve characteristics

Quantity	Certified value ¹⁾	Uncertainty ²⁾	Unit
y_1 ³⁾	158,1	7,3	mm ³ g ⁻¹
y_2 ⁴⁾	0,5021	0,028	MPa
y_3 ⁵⁾	0,2616	0,039	MPa
p_{50}	0,4795	0,029	MPa
d_{50}	3,074	0,19	μm

¹⁾ Mercury intrusion curves from the designed interlaboratory testing were analysed by means of a multivariate variance components model for the curve characteristics y_1 , y_2 and y_3 . The results were mean curve characteristics (certified values) and prediction intervals for the curve characteristics. Adjusted curves and statistics from the variance components model were used to create a certified pressure volume curve with a prediction band.

²⁾ Half-width of the prediction interval resulting from the variance analytical investigation of the pressure volume curve characteristics y_1 , y_2 , and y_3 at the significance level 0,95.

³⁾ y_1 : Intruded volume at the saturation point 1,55 MPa (saturation value).

⁴⁾ y_2 : Pressure at 57,5 % of the saturation value. This value has been determined by local polynomial estimation (Epanechnikov kernel with band width $h = 0,025$ MPa).

⁵⁾ y_3 : Difference of the pressures at which the intrusion curve has got 87,5 % and 25 % respectively of the saturation value.

BAM-P126**Mercury intrusion curve between 0,55 MPa and 2,1 MPa**

Flat membrane

Mercury intrusion curve characteristics

Quantity	Certified value ¹⁾	Uncertainty ²⁾	Unit
y_1 ³⁾	110,9	8,5	mm ³ g ⁻¹
y_2 ⁴⁾	0,8682	0,0408	MPa
y_3 ⁵⁾	0,2965	0,0305	MPa
p_{50}	0,8441	0,0416	MPa
d_{50}	1,746	0,086	μm

¹⁾ Mercury intrusion curves from the designed interlaboratory testing were analysed by means of a multivariate variance components model for the curve characteristics y_1 , y_2 and y_3 . The results were mean curve characteristics (certified values) and prediction intervals for the curve characteristics. Adjusted curves and statistics from the variance components model were used to create a certified pressure volume curve with a prediction band.

²⁾ Half-width of the prediction interval resulting from the variance analytical investigation of the pressure volume curve characteristics y_1 , y_2 , and y_3 at the significance level 0,95.

³⁾ y_1 : Intruded volume at the saturation point 2,1 MPa (saturation value).

⁴⁾ y_2 : Pressure at 57,5 % of the saturation value. This value has been determined by local polynomial estimation (Epanechnikov kernel with band width $h = 0,05$ MPa).

⁵⁾ y_3 : Difference of the pressures at which the intrusion curve has got 87,5 % and 25 % respectively of the saturation value.

BAM-P128

Porosity properties of macroporous alumina ceramic calculated from the mercury intrusion up to a maximum pressure between 0,2 and 0,4 MPa

Property	Certified value ^{a)}	Uncertainty ^{b)}	Unit
Specific pore volume ^{c)} V_p	220	6	mm ³ g ⁻¹
Median pore diameter ^{d)} d_{50}	27,6	1,0	μm
Informative value			
Density ρ_s	3,6405	0,0019	g/cm ³

^{a)} Mean value of the means of accepted data sets each derived from at least 19 single values.

^{b)} Uncertainty $U = k \cdot u_c$ calculated according to ISO Guide 35 and ISO/IEC Guide 98 with the coverage factor $k=2$ (giving a level of confidence of approximately 95 %). The combined standard uncertainty u_c of each certified property includes uncertainty contributions resulting from the interlaboratory testing, the study of inhomogeneities and stability of the material.

^{c)} Specific pore volume V_p calculated from the mercury intrusion with maximum pressure in a low-pressure device. Described in ISO 15901-1 and DIN 66133.

^{d)} Median pore diameter d_{50} calculated according to the Washburn equilibrium model as described in ISO 15901-1 and DIN 66133.

Layer and surface reference materials

EDS-TM002 test material and optional software package for the performance check of an energy dispersive X-ray spectrometer (EDS)

The test material EDS-TM002 (2nd generation) together with an accompanying software package, “EDX spectrometer check”, have been made available in 2009 by BAM [1] to be employed by EDS users to check the performance of an EDS attached to a SEM. Particularly for test laboratories operating under accreditation schemes like ISO/IEC 17025, a periodical control of the critical instrumental parameters in end-user laboratories is required.

With EDS-TM002 test material, this periodical check is simplified to the acquisition of only one 10 kV spectrum. The software “EDX spectrometer check” is destined to evaluate automatically this spectrum and determine the performance of the EDS in terms of energy resolution and calibration, as well as possible alteration of low-energy efficiency due to detector contamination. The energy resolution can be compared with the specified values according to the standard ISO 15632:2012 [2].

EDS-TM is a synthetic material consisting of a 6 µm thick layer of C, Al, Mn, Cu and Zr deposited on a silicon substrate. The chemical composition of EDS-TM was chosen such as to give nearly equal intensities of the low energy lines in a 10 kV spectrum, see **Figure 1**, thus, making it very sensitive against spectrometer efficiency changes. A detailed description of the test material and software together with examples of application can be found in [3,4].

When the FWHM of the X-ray lines in the EDS-TM spectrum are determined, the spectrum background must be subtracted accurately. The applied physical background subtraction procedure is robust and considers the transmission of the detector window [3]. The new software version 3.6, released in December 2018 [4], includes selection of silicon nitride window (with a transmission according to [5]) and the case of windowless detector. Moreover, the new version allows importing of spectra in Bruker spx-format and EMSA/MSA files from EDAX TEAM software.

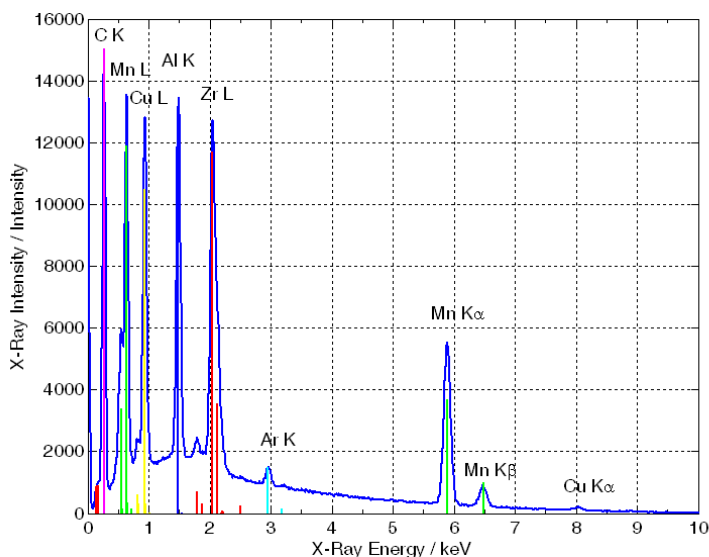


Figure 1: 10 kV X-ray spectrum of EDS-TM002, DVD with the evaluation software EDX Spectrometer Test (version 3.6, Release Dec. 2018) and photo of the test material.

Figure 2 displays the results of the performance check of an SDD EDS spectrometer with a silicon nitride window as provided by the updated “EDS Spectrometer Test” software (version 3.6). The high Mn $L\alpha$ /Mn $K\alpha$ intensity ratio should be noticed.

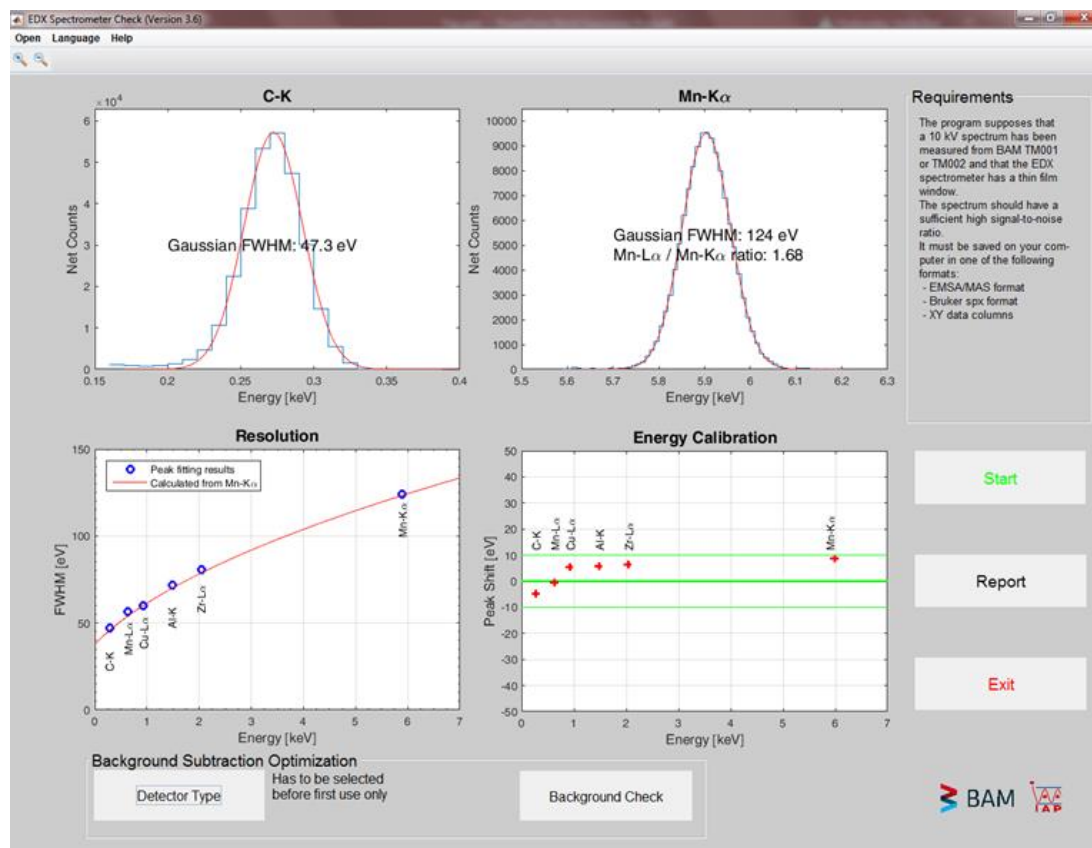


Figure 2: Result of evaluation of an SDD EDS with silicon nitride window with the updated software package “EDS Spectrometer Test”, version 3.6 (release 2018).

- [1] M Procop and V-D Hodoroaba, Microsc. Microanal. 15 (S2) (2009) 1120
- [2] ISO 15632:2012 "Microbeam Analysis – Selected instrumental performance parameters for the specification and checking of energy-dispersive X-ray spectrometers for use in electron probe microanalysis". (Geneva, Switzerland: ISO – International Standards Organization)
- [3] V-D Hodoroaba and M Procop, Microsc. Microanal. 20 (2014) 1556
- [4] V-D Hodoroaba, R Terborg and M Procop, Microsc. Microanal. 24 (S1) (2018) 730
- [5] <http://amptek.com/products/c-series-low-energy-x-ray-windows/#4>

Particle size distribution

**CRM for particle size distribution by laser diffraction methods
according to ISO 13320**

BAM-D001

Description: hexagonal silicon carbide powder

Year of issue: 2012

Certified properties:

Specific particle diameter corresponding to the cumulative undersize volume distribution Q3	Equivalent spherical diameter ¹⁾	Uncertainty ²⁾
	μm	μm
d_{10}	7,02	0,25
d_{50}	12,48	0,21
d_{90}	20,8	1,1

¹⁾ The certified value is the weighted mean of 13 laboratory means which participated in the interlaboratory comparison for certification according to ISO 13320:2009.

²⁾ Estimated expanded uncertainty with a coverage factor of $k=2$, corresponding to a level of confidence of about 95%, as defined in the Guide to the Expression of Uncertainty in Measurement (GUM, ISO/IEC Guide 98-3:2008).

Values for information:

Refractive index n_p ³⁾	2,645
Imaginary part k_p of particles' refractive index (absorption) ³⁾	0,1
Density ρ in g/ cm ³	3,205

³⁾ Wavelength: 633 nm

Polymeric reference materials

CRMs for the determination of the molecular weight

CRM-No.	ERM®-FA001 (BAM-P001)	ERM®-FA002 (BAM-P002)	BAM-P011	BAM-P012
Description	Polystyrene	Polystyrene	Polystyrene	Polystyrene
	Amorphous material	Pellets	Pellets	Pellets
Year of issue	2002	2002	2007	2007
Weight-average molecular weight (M_w) by <u>light scattering (LS)</u> g/mol	87600 ± 2245	205600 ± 3075	286000 ± 4000	348000 ± 8000
Weight-average molecular weight (M_w) by Size Exclusion Chromatography (SEC) g/mol	–	–	284000 ± 9000	343000 ± 12000
Intrinsic viscosity by <u>viscometry</u> mL/g	42,37 ± 0,83	68,38 ± 0,79	88,73 ± 0,80	104,0 ± 1,8

Note: Estimated expanded uncertainty with a coverage factor of $k=2$.

The reference materials are intended for the calibration of instruments for the determination of the molecular weight and molecular weight distribution of polymers.

Microplastic

BAM-P201, Artificially aged Polyethylene (PE)

	Particle size in μm	Standard deviation in μm	Rel. standard deviation in %
d₁₀	17,9	0,3	1,8
d₅₀	61,2	1,4	2,3
d₉₀	158,6	7,5	4,7

Carbonyl-Index	Standard deviation	Rel. standard deviation in %
1,86	0,12	6,7

ΔH in $\mu\text{W}/\text{mg}$	Standard deviation in $\mu\text{W}/\text{mg}$	Rel. standard deviation in %
12360	1012	8,2

BAM-P202, Polystyrene (PS)

	Particle size in μm	Twofold Standard deviation 2·s in μm	Expanded uncertainty in μm
d₁₀	91	9	13
d₅₀	206	27	29
d₉₀	311	28	28

BAM-P206, Polyethylenterephthalat (PET)

	Particle size in μm	Twofold Standard deviation 2·s in μm	Expanded uncertainty in μm
d₁₀	29	1	2
d₅₀	62	1	4
d₉₀	107	3	8

Isotopic reference materials

CRMs certified for the isotopic composition of boron

Certified quantity: Isotopic composition of boron in an aqueous solution of boric acid, certified with expanded relative uncertainties of less than 0,12 %.

Application: Calibration and validation of ICP-MS procedures used for the determination of boron isotope amount ratios. Boron isotope amount ratios have to be determined within the surveillance of the primary cooling circuit in nuclear power plants equipped with a pressurized water reactor. They also have to be determined in container materials, which are doped with boron serving as a neutron shield. ERM®-AE124 may also be used for isotope tracer studies and as spike for isotope dilution analysis. In the latter case, however, the characterization of the boron mass fraction by reverse IDMS at the time of use might be advisable, when low measurement uncertainties (<1 % relative) are aimed at.

CRM-No.	ERM®-AE102a	ERM®-AE104a	ERM®-AE123	ERM®-AE124
Isotope abundance ratio $R(^{10}\text{B}/^{11}\text{B})$	0,4285 (6)	0,4596 (6)	0,2474 (4)	24,04 (4)
Isotope abundance ratio $R(^{11}\text{B}/^{10}\text{B})$	2,3338 (30)	2,1758 (28)	4,042 (6)	0,04160 (6)
Isotope abundance ^{10}B ^{11}B	0,29995 (27) 0,70005 (27)	0,31488 (28) 0,68512 (28)	0,19832 (22) 0,80168 (22)	0,96006 (6) 0,03994 (6)
Molar mass $M(\text{B})$ in $\text{g}\cdot\text{mol}^{-1}$	10,71044 (27)	10,69557 (28)	10,81170 (22)	10,05273 (6)
	Informative value			
Mass fraction in solution $w(\text{B})$ in $\text{mg}\cdot\text{kg}^{-1}$	999 (20)	1000 (20)	1063 (106)	1002 (20)

All uncertainties indicated are expanded uncertainties $U=k\cdot u$ where $k=2$ and u is the combined standard uncertainty calculated according EURACHEM and ISO guidelines. They are given in parentheses and apply to the last one or two digits of the value.

CRM-No.	ERM®-AE101a	
	Certified value	Uncertainty
Isotope amount ratio $n(^{10}\text{B})/n(^{11}\text{B})$ in mol/mol	0,28212	0,00038
Isotope amount ratio $n(^{11}\text{B})/n(^{10}\text{B})$ in mol/mol	3,5446	0,0048
Isotope amount fraction $n(^{10}\text{B})/n(\text{B})$ in mol/mol	0,22004	0,00023
Isotope amount fraction $n(^{11}\text{B})/n(\text{B})$ in mol/mol	0,77996	0,00023
Mass fraction of B in solution $M(\text{B})$ in mol/mol	10,79007	0,00023
	Informative value	
Mass fraction of B in $\text{mg}\cdot\text{kg}^{-1}$	1026	21

Certified quantity: $\delta^{11}\text{B}$ relative to NIST SRM 951: $\delta^{11}\text{B}$ is a measure for the isotope variation. It is expressed as the shift of the isotopic composition relative to an internationally accepted standard given in per mill. It is calculated according to the following equation, with NIST SRM 951 (isotope reference material for boron) being used as reference: $\delta^{11}\text{B} = ((R_{\text{sample}}/R_{\text{reference}})-1)$. This certified reference material is traceable to the international δ -scale for boron with the origin being represented by NIST SRM 951.

Application: Isotope reference materials are essential to enable the determination of reliable and comparable isotope data. Besides the correction of mass fractionation or mass discrimination isotope reference materials are indispensable for validation and quality control of analytical procedures. In general δ -values of specific elements express the difference of an isotope ratio of a sample relative to an international accepted standard in per mill. Such δ -values are used in science and technology to study geochemical and environmental processes and to determine the provenance of food and the origin of forensic and archaeological artefacts.

These three boron isotope reference materials are certified for their $\delta^{11}\text{B}$ -values relative to NIST SRM 951 which is the internationally accepted origin of the δ -scale for boron. The certified $\delta^{11}\text{B}$ values cover about three-quarters of the known natural boron isotope variability. The $\delta^{11}\text{B}$ reference materials are primarily intended to be used for quality control and the validation of chemical and mass spectrometric procedures.

CRM-No.	ERM®-AE120		ERM®-AE122	
$\delta^{11}\text{B}_{\text{NIST 951}}$ in ‰	-20,2	(0,6)	39,7	(0,6)
	Informative value			
Isotope abundance ratio $R(^{10}\text{B}/^{11}\text{B})$	0,25236	(33)	0,23782	(31)
Isotope abundance ratio $R(^{11}\text{B}/^{10}\text{B})$	3,963	(6)	4,205	(6)
Isotope abundance ^{10}B	0,20150	(21)	0,19213	(20)
	0,79850	(21)	0,80787	(20)
Molar mass $M(\text{B})$ in $\text{g}\cdot\text{mol}^{-1}$	10,80853	(21)	10,81787	(20)
Mass fraction in solution $w(\text{B})$ in $\text{mg}\cdot\text{kg}^{-1}$	100,0	(2,0)	100,0	(2,0)

All uncertainties indicated are expanded uncertainties $U=k\cdot u$ where $k=2$ and u is the combined standard uncertainty calculated according EURACHEM and ISO guidelines. They are given in parentheses and apply to the last one or two digits of the value.

CRM-No.	ERM®-AE121		ERM®-AE125	
	Certified value	Uncertainty	Certified value	Uncertainty
$\delta^{11}\text{B}_{\text{NIST 951}}$ in ‰	19,9	0,6	-124,00	0,48
	Informative value			
Isotope amount ratio $n(^{10}\text{B})/n(^{11}\text{B})$ in mol/mol	0,24233	0,00032	0,28212	0,00038
Isotope amount ratio $n(^{11}\text{B})/n(^{10}\text{B})$ in mol/mol	4,127	0,006	3,5446	0,0048
Isotope amount fraction $n(^{10}\text{B})/n(\text{B})$ in mol/mol	0,19506	0,00021	0,22004	0,00023
Isotope amount fraction $n(^{11}\text{B})/n(\text{B})$ in mol/mol	0,80494	0,00021	0,77996	0,00023
Molar mass of B in solution $M(\text{B})$ in g/mol	10,81495	0,00021	10,79007	0,00023
Mass fraction of B in solution $M(\text{B})$ in mol/mol	100,0	2,0	101,4	2,0

CRM certified for the isotopic composition of cadmium

Certified quantity: Primary isotopic reference material certified for the isotopic composition of cadmium in a dilute nitric acid solution with expanded relative uncertainties of less than 0,07 %.

Application: Calibration of any kind of mass spectrometric procedures used for the determination of cadmium isotope amount ratios. BAM-I012 represents the best measurement for cadmium isotope amount ratios as approved by IUPAC. Additionally, BAM-I012 defines the delta-scale for $\delta^{114/110}\text{Cd}$ measurements.

CRM-No.	BAM-I012	
Isotope amount ratios in $\text{mol}\cdot\text{mol}^{-1}$		
$n(^{106}\text{Cd})/n(^{111}\text{Cd})$	0,09751	(7)
$n(^{108}\text{Cd})/n(^{111}\text{Cd})$	0,06951	(3)
$n(^{110}\text{Cd})/n(^{111}\text{Cd})$	0,97504	(10)
$n(^{112}\text{Cd})/n(^{111}\text{Cd})$	1,8835	(4)
$n(^{113}\text{Cd})/n(^{111}\text{Cd})$	0,95479	(16)
$n(^{114}\text{Cd})/n(^{111}\text{Cd})$	2,2437	(7)
$n(^{116}\text{Cd})/n(^{111}\text{Cd})$	0,58583	(26)
Isotope amount fractions in $\text{mol}\cdot\text{mol}^{-1}$		
$n(^{106}\text{Cd})/n(\text{Cd})$	0,012485	(9)
$n(^{108}\text{Cd})/n(\text{Cd})$	0,008901	(4)
$n(^{110}\text{Cd})/n(\text{Cd})$	0,124846	(16)
$n(^{111}\text{Cd})/n(\text{Cd})$	0,128043	(13)
$n(^{112}\text{Cd})/n(\text{Cd})$	0,24117	(4)
$n(^{113}\text{Cd})/n(\text{Cd})$	0,122254	(22)
$n(^{114}\text{Cd})/n(\text{Cd})$	0,28729	(6)
$n(^{116}\text{Cd})/n(\text{Cd})$	0,07501	(4)
Molar mass $M(\text{Cd})$ in $\text{g}\cdot\text{mol}^{-1}$	112,41218	(18)
	Informative value	
Mass fraction in solution $w(\text{Cd})$ in $\text{mg}\cdot\text{kg}^{-1}$	994	(5)

All uncertainties indicated are expanded uncertainties $U=k\cdot u$ where $k=2$ and u is the combined standard uncertainty calculated according EURACHEM and ISO guidelines, excepting for $w(\text{Cd})$, where $k=4.5$. They are given in parentheses and apply to the last one or two digits of the value.

CRM certified for the mass fraction and the isotopic composition of palladium

Certified quantity: Spike isotopic reference material certified for the mass fraction of ^{106}Pd and the isotopic composition of palladium in 20 % hydrochloric acid with expanded relative uncertainties of 0,24 % for the mass fraction of ^{106}Pd .

Application: The spike isotopic reference material ERM®-AE140 is a solution of isotopically enriched Pd in 20 % hydrochloric acid and filled in flame-sealed quartz ampoules containing approximately 7 mL solution. This material is designed to serve as isotopically enriched analogue or so-called spike in Isotope Dilution Mass Spectrometry (IDMS) for the quantification of Pd.

CRM-No.	ERM®-AE140	
Mass fraction $w(^{106}\text{Pd})$ in $\text{mg}\cdot\text{kg}^{-1}$	20,24	(5)
Isotope amount ratios in $\text{mol}\cdot\text{mol}^{-1}$ $n(^{102}\text{Pd})/n(^{106}\text{Pd})$ $n(^{104}\text{Pd})/n(^{106}\text{Pd})$ $n(^{105}\text{Pd})/n(^{106}\text{Pd})$ $n(^{108}\text{Pd})/n(^{106}\text{Pd})$ $n(^{110}\text{Pd})/n(^{106}\text{Pd})$	0,0000791 0,001247 0,007518 0,004785 0,001156	(11) (11) (30) (22) (11)
Indicative values		
Mass fraction $w(\text{Pd})$ in $\text{mg}\cdot\text{kg}^{-1}$	20,54	(5)
Isotope amount fractions in $\text{mol}\cdot\text{mol}^{-1}$ $n(^{102}\text{Pd})/n(\text{Pd})$ $n(^{104}\text{Pd})/n(\text{Pd})$ $n(^{105}\text{Pd})/n(\text{Pd})$ $n(^{106}\text{Pd})/n(\text{Pd})$ $n(^{108}\text{Pd})/n(\text{Pd})$ $n(^{110}\text{Pd})/n(\text{Pd})$	0,0000780 0,001229 0,007408 0,98543 0,004716 0,001139	(10) (10) (30) (5) (22) (11)
Molar mass $M(\text{Pd})$ in $\text{g}\cdot\text{mol}^{-1}$	105,907312	(75)

All uncertainties indicated are expanded uncertainties $U=k\cdot u$ where $k=2$ and u is the combined standard uncertainty calculated according EURACHEM and ISO guidelines. They are given in parentheses and apply to the last one or two digits of the value.

CRM certified for the mass fraction and the isotopic composition of platinum

Certified quantity: Spike isotopic reference material certified for the mass fraction of ^{194}Pt and the isotopic composition of platinum in 20 % hydrochloric acid with expanded relative uncertainties of 0,61 % for the mass fraction of ^{194}Pt .

Application: The spike isotopic reference material ERM®-AE141 is a solution of isotopically enriched Pt in 20 % hydrochloric acid and filled in flame-sealed quartz ampoules containing approximately 7 mL solution. This material is designed to serve as isotopically enriched analogue or so-called spike in Isotope Dilution Mass Spectrometry (IDMS) for the quantification of Pt.

CRM-No.	ERM®-AE141	
Mass fraction $w(^{194}\text{Pt})$ in $\text{mg}\cdot\text{kg}^{-1}$	18,18	(11)
Isotope amount ratios in $\text{mol}\cdot\text{mol}^{-1}$ $n(^{190}\text{Pt})/n(^{194}\text{Pt})$ $n(^{192}\text{Pt})/n(^{194}\text{Pt})$ $n(^{195}\text{Pt})/n(^{194}\text{Pt})$ $n(^{196}\text{Pt})/n(^{194}\text{Pt})$ $n(^{198}\text{Pt})/n(^{194}\text{Pt})$	0,0000012 (6) 0,000342 (4) 0,0739 (8) 0,01749 (21) 0,002022 (29)	
Indicative values		
Mass fraction $w(\text{Pt})$ in $\text{mg}\cdot\text{kg}^{-1}$	19,90	(12)
Isotope amount fractions in $\text{mol}\cdot\text{mol}^{-1}$ $n(^{190}\text{Pt})/n(\text{Pt})$ $n(^{192}\text{Pt})/n(\text{Pt})$ $n(^{194}\text{Pt})/n(\text{Pt})$ $n(^{195}\text{Pt})/n(\text{Pt})$ $n(^{196}\text{Pt})/n(\text{Pt})$ $n(^{198}\text{Pt})/n(\text{Pt})$	0,0000011 (6) 0,000312 (4) 0,9143 (8) 0,0676 (6) 0,01599 (26) 0,001849 (10)	
Molar mass $M(\text{Pt})$ in $\text{g}\cdot\text{mol}^{-1}$	194,0692	(10)

All uncertainties indicated are expanded uncertainties $U=k\cdot u$ where $k=2$ and u is the combined standard uncertainty calculated according EURACHEM and ISO guidelines. They are given in parentheses and apply to the last one or two digits of the value.

CRM certified for the isotopic composition of lead

Certified quantity: isotopic reference material certified for the isotopic composition of lead in a dilute nitric acid solution and in bronze with expanded relative uncertainties of $\leq 0,1\%$.

Application: Calibration and validation of any kind of mass spectrometric procedures used for the determination of lead isotope amount ratios.

Isotope reference materials are essential to enable the determination of reliable and comparable isotope data. Besides the correction of mass fractionation or mass discrimination isotope reference materials are indispensable for validation and quality control of analytical procedures. ERM®-EB400 is the first matrix reference material certified for the Pb isotopic composition. It is best suited to calibrate and validate any Pb isotope ratio determination in metals. It helps especially for validating Pb-matrix separation procedures. Fields of application are analytical chemistry, archaeometry, geochemistry and others.

CRM-No.	ERM®-AE142	ERM®-EB400
Isotope amount ratios in $\text{mol}\cdot\text{mol}^{-1}$		
$n(^{206}\text{Pb})/n(^{204}\text{Pb})$	21,114 (17)	18,072 (17)
$n(^{207}\text{Pb})/n(^{204}\text{Pb})$	15,944 (17)	15,578 (18)
$n(^{208}\text{Pb})/n(^{204}\text{Pb})$	39,850 (44)	38,075 (46)
$n(^{206}\text{Pb})/n(^{204}\text{Pb})$	1,8874 (10)	2,1068 (14)
Isotope amount fractions in $\text{mol}\cdot\text{mol}^{-1}$		
$n(^{204}\text{Pb})/n(\text{Pb})$	0,012 8357 (83)	0,013 7504 (98)
$n(^{206}\text{Pb})/n(\text{Pb})$	0,271 01 (23)	0,248 50 (24)
$n(^{207}\text{Pb})/n(\text{Pb})$	0,204 65 (21)	0,214 20 (24)
$n(^{208}\text{Pb})/n(\text{Pb})$	0,511 50 (32)	0,523 55 (35)
Molar mass $M(\text{Pb})$ in $\text{g}\cdot\text{mol}^{-1}$	207,177 83 (53)	207,209 68 (57)
	Informative value	Additional material information
Mass fraction in solution $w(\text{Pb})$ in $\text{mg}\cdot\text{kg}^{-1}$	100,0 (2,0)	44,9 (2,3)

All uncertainties indicated are expanded uncertainties $U=k\cdot u_c$ where $k=2$ and u_c is the combined standard uncertainty calculated according EURACHEM and ISO guidelines. They are given in parentheses and apply to the last one or two digits of the value.

CRM certified for the isotopic composition of magnesium

Certified quantity: Primary isotopic reference materials certified for the isotopic composition of magnesium in a dilute nitric acid solution with relative expanded uncertainties of less than 0,035 %.

Application: Calibration of any kind of mass spectrometric procedures used for the determination of magnesium isotope amount ratios. ERM-AE143, ERM-AE144 and ERM-AE145 represent the best measurement for magnesium isotope amount ratios as approved by IUPAC. ERM-AE143 additionally is designed to anchor the magnesium delta-scale at $\delta^{26/24}\text{Mg} = 0$.

CRM-No.	ERM-AE143	ERM-AE144	ERM-AE145
Isotope amount ratios in $\text{mol}\cdot\text{mol}^{-1}$ $n(^{25}\text{Mg})/n(^{24}\text{Mg})$ $n(^{26}\text{Mg})/n(^{24}\text{Mg})$	0,126 590 (20) 0,139 362 (43)	0,126 486 (22) 0,139 138 (39)	0,126 514 (16) 0,139 185 (29)
Isotope amount fractions in $\text{mol}\cdot\text{mol}^{-1}$ $n(^{24}\text{Mg})/n(\text{Mg})$ $n(^{25}\text{Mg})/n(\text{Mg})$ $n(^{26}\text{Mg})/n(\text{Mg})$	0,789 920 (46) 0,099 996 (14) 0,110 085 (28)	0,790 124 (39) 0,099 939 (13) 0,109 936 (25)	0,790 078 (28) 0,099 956 (10) 0,109 967 (21)
Molar mass $M(\text{Mg})$ in $\text{g}\cdot\text{mol}^{-1}$	24,305 017 (73)	24,304 664 (63)	24,304 741 (46)
	Informative value	Informative value	Informative value
Mass fraction in solution $w(\text{Mg})$ in $\text{mg}\cdot\text{kg}^{-1}$	50.0 (1.0)	50.0 (1.0)	50.0 (1.0)

All uncertainties indicated are expanded uncertainties $U = k \cdot u_c$, where $k = 2$ and u_c is the combined standard uncertainty calculated according EURACHEM and ISO guidelines. They are given in parentheses and apply to the last one or two digits of the value.

Nano materials

BAM-N008

Size distribution and concentration of silver nanoparticles calculated from
small-angle X-ray scattering (SAXS)

	Value ¹	Uncertainty ² <i>U</i>	Certified ³	Unit
Diameter (<i>D</i>)	5.8	0.5 (7%)	yes	nm
Size distribution width (σ)	1.33	0.18 (13%)	no	nm
Number density (<i>N</i>)	3.7	0.7 (18%)	yes	10 ⁻⁶ mol l ⁻¹
Concentration (<i>c</i>)	3.0	0.5 (16%)	no	g l ⁻¹

BAM-N012

Particle size of iron oxide nanocubes determined by transmission electron microscopy and
Small-angle X-ray scattering

Characteristics determined by TEM	Value	Uncertainty <i>U</i>
Median Area Equivalent Circular Diameter	9.1 nm	0.8 nm
Median Area Equivalent Square Edge Length	8.1 nm	0.7 nm

Experts

Iron and steel products**Non ferrous metals****Pure substances****Special materials**

Dr. Sebastian Recknagel

phone: +49 (0)30 8104-1111
fax: +49 (0)30 8104-71111
email: sebastian.recknagel@bam.de

Dr. Markus Ostermann

phone: +49 (0)30 8104-1143
fax: +49 (0)30 8104-71143
email: markus.ostermann@bam.de

Environment

Dr. Matthias Koch
(organic analytes)

phone: +49 (0)30 8104-1170
fax: +49 (0)30 8104-71170
email: matthias.koch@bam.de

Dr. Sebastian Recknagel
(inorganic analytes)

phone: +49 (0)30 8104-1111
fax: +49 (0)30 8104-71111
email: sebastian.recknagel@bam.de

Food, consumer products

Dr. Matthias Koch

phone: +49 (0)30 8104-1170
fax: +49 (0)30 8104-71170
email: matthias.koch@bam.de

Primary reference gas mixtures

Dr. Heinrich Kipphardt

phone: +49 (0)30 8104-1116
fax: +49 (0)30 8104-74581
email: gasanalytik@bam.de

Elastomeric materials

Dietmar Schulze

phone: +49 (0)30 8104-3340
email: crm-elastomer@bam.de

X-ray film step tablet

Dr. Uwe Zscherpel

phone: +49 (0)30 8104-3677
fax: +49 (0)30 8104-73677
email: uwe.zscherpel@bam.de

Porous reference materials

Carsten Prinz

phone: +49 (0)30 8104-5524
fax: +49 (0)30 8104-75524
email: porosimetry@bam.de

Dr. Franziska Emmerling

phone: +49 (0)30 8104-1133
fax: +49 (0)30 8104-71133
email: porosimetry@bam.de

Spectral fluorescence standards

Dr. Ute Resch-Genger

phone: +49 (0)30 8104-1134
fax: +49 (0)30 8104-71134
email: ute.resch@bam.de

Layer and surface reference materials

Dr. Vasile-Dan Hodoroaba

phone: +49 (0)30 8104-3144
fax: +49 (0)30 8104 73144
email: dan.hodoroaba@bam.de

Particle size distribution

Petra Kuchenbecker

phone: +49 (0)30 8104-4816
fax: +49 (0)30 8104-74816
email: petra.kuchenbecker@bam.de

Polymeric reference materials

Dr. Steffen Weidner

phone: +49 (0)30 8104-1633
fax: +49 (0)30 8104-71633
email: steffen.weidner@bam.de

Isotopic reference materials

Dr. Jochen Vogl

phone: +49 (0)30 8104-1144
fax: +49 (0)30 8104-71144
email: jochen.vogl@bam.de

Nano materials

Dr. Harald Bresch

phone: +49 (0)30 8104-3364
fax: +49 (0)30 8104-73364
email: harald.bresch@bam.de